


# FRED PA-1

## Automated External Defibrillator (AED)



### User Guide

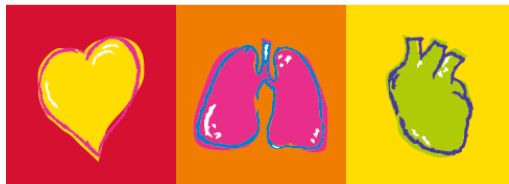

**SCHILLER**

The Art of Saving Lives

### Sales and service information

The SCHILLER sales and service centre network is world-wide. For the address of your local distributor, contact your nearest SCHILLER subsidiary.

In case of difficulty, a complete list of all distributors and subsidiaries is provided on our internet site:

<http://www.schiller.ch>

Sales information can also be obtained from:

[sales@schiller.ch](mailto:sales@schiller.ch)



#### Manufacturer

SCHILLER MEDICAL  
4, rue Louis Pasteur  
F- 67160 Wissembourg

Phone +33 3 88 63 36 00  
Fax +33 3 88 94 12 82  
E-mail: [info@schiller.fr](mailto:info@schiller.fr)  
Web: [www.schiller-medical.fr](http://www.schiller-medical.fr)

Art. no./revision	Date	Note
0-48-0240j	2025-06-16	Update according to Specification and validation
0-48-0240k	2026-02-16	Update according to Specifications and add the child adapter



The **FRED PA-1** bears the CE-0459 mark (Notified Body GMED), indicating its compliance with the general safety and performance requirements of Annex I of the Medical Device Regulation (EU) 2017/745 regarding safety, functionality and labelling. The requirements apply to patients, users and third persons who come into contact with this device within the scope of its intended use. First declaration 2025-02-20.

The summary of safety and clinical performance is available on the EUDAMED website.

Article no: 0-48-0240 Rev. k  
Original  
Issue date: 2026-02-16  
Corresponds to the original  
Software: ≥ 05



**SCHILLER**  
The Art of Saving Lives

# Table of Contents

<b>1</b>	<b>Safety Notes .....</b>	<b>7</b>
1.1	<b>User Profiles .....</b>	<b>7</b>
1.2	<b>Intended Use .....</b>	<b>7</b>
1.2.1	General intended purpose.....	7
1.2.2	General warnings and precautions for use .....	8
1.2.3	Defibrillation function.....	10
1.3	<b>Medical Indications .....</b>	<b>11</b>
1.4	<b>Clinical Benefits.....</b>	<b>11</b>
1.5	<b>Contraindication for Use.....</b>	<b>11</b>
1.6	<b>Operation with other Devices .....</b>	<b>12</b>
1.7	<b>Maintenance and Cleaning .....</b>	<b>12</b>
1.8	<b>Known Side Effects .....</b>	<b>12</b>
1.9	<b>General Notes for FRED PA-1 .....</b>	<b>12</b>
1.10	<b>Cybersecurity.....</b>	<b>13</b>
1.10.1	Networks and internet .....	13
1.10.2	Patient data (personal data).....	13
1.10.3	Setup security guidance.....	13
1.11	<b>Additional Terms .....</b>	<b>14</b>
1.11.1	Implied authorisation .....	14
1.11.2	Terms of warranty .....	14
1.11.3	Reporting security incidents and vulnerability disclosure policy.....	14
1.12	<b>Symbols and Indicators .....</b>	<b>15</b>
1.12.1	Symbols used in this user guide .....	15
1.12.2	Symbols used on the <b>FRED PA-1</b> .....	16
1.12.3	Symbols used on the batteries.....	17
1.12.4	Symbols used on the electrode packaging .....	18
1.12.5	Symbols specific to the child adapter.....	20
<b>2</b>	<b>Components and Operation .....</b>	<b>21</b>
2.1	<b>General Information .....</b>	<b>21</b>
2.2	<b>Design.....</b>	<b>22</b>
2.2.1	General design.....	22
2.2.2	Available versions .....	23
2.3	<b>Operating and Display Elements .....</b>	<b>24</b>
2.3.1	<b>FRED PA-1</b> overview .....	24
2.3.2	Operating elements.....	25
2.4	<b>Function .....</b>	<b>26</b>
2.4.1	Automatic self-test.....	26
2.4.2	Defibrillation procedure .....	27
<b>3</b>	<b>Initial Operation .....</b>	<b>28</b>
3.1	<b>General Information and Safety Notes .....</b>	<b>28</b>
3.2	<b>Inserting the Battery.....</b>	<b>29</b>
3.3	<b>Adding Emergency Number Stickers .....</b>	<b>29</b>
3.4	<b>Attach the child adapter (if applicable) .....</b>	<b>30</b>

<b>3.5</b>	<b>Switching the FRED PA-1 On/Off .....</b>	<b>31</b>
<b>3.6</b>	<b>Battery Monitoring .....</b>	<b>32</b>
3.6.1	Sufficient battery capacity .....	32
3.6.2	Low battery capacity indication .....	32
3.6.3	Battery depleted during use, limited mode CPR .....	33
<b>3.7</b>	<b>Replacing the pre-connected Pads and child adapter ....</b>	<b>34</b>
3.7.1	Expired pads .....	34
3.7.2	Connect the electrodes .....	34
3.7.3	Child adapter .....	35
3.7.4	Connect the electrodes with the child adapter .....	35
<b>4</b>	<b>Defibrillation .....</b>	<b>36</b>
<b>4.1</b>	<b>Instructions and Safety Notes .....</b>	<b>36</b>
4.1.1	Instructions .....	36
4.1.2	Safety notes for defibrillation use .....	37
4.1.3	Defibrillating child and infant patients .....	39
<b>4.2</b>	<b>Application of the Adhesive Electrodes .....</b>	<b>41</b>
4.2.1	General information .....	41
4.2.2	Unpacking the electrodes .....	42
4.2.3	Applying the electrodes .....	43
4.2.4	Connect the adult electrodes with the child adapter .....	45
4.2.5	Checking the electrodes .....	45
4.2.6	Checking the child adapter .....	46
<b>4.3</b>	<b>Semi-automatic Defibrillation .....</b>	<b>47</b>
<b>4.4</b>	<b>Automatic Defibrillation .....</b>	<b>50</b>
4.4.1	Functional description of automatic AEDs .....	50
4.4.2	Safety notes for automatic defibrillation .....	50
4.4.3	Automatic defibrillation procedure .....	51
<b>4.5</b>	<b>Internal Safety Discharge .....</b>	<b>54</b>
<b>4.6</b>	<b>Finishing the Therapy .....</b>	<b>54</b>
<b>4.7</b>	<b>Replacing the Battery .....</b>	<b>55</b>
<b>5</b>	<b>Communication .....</b>	<b>56</b>
<b>5.1</b>	<b>Retrieving Intervention Data .....</b>	<b>56</b>
5.1.1	For standard FRED PA-1 with an SD card .....	56
5.1.2	For FRED PA-1 equipped with a cellular network .....	57
<b>6</b>	<b>Maintenance .....</b>	<b>58</b>
<b>6.1</b>	<b>Maintenance Intervals .....</b>	<b>58</b>
6.1.1	Device status file .....	59
6.1.2	Service and shelf life .....	59
6.1.3	Visual inspection of the <b>FRED PA-1</b> and accessories .....	60
6.1.4	RTU LED .....	61
6.1.5	Maintenance of the non-rechargeable Li/MnO2 battery .....	61
<b>6.2</b>	<b>Cleaning and Disinfecting .....</b>	<b>62</b>
6.2.1	Cleaning detergents .....	62
6.2.2	Disinfection .....	62
6.2.3	Cleaning and disinfecting the FRED PA-1, cable, adapter and sensor .....	63

<b>6.3</b>	<b>Order Information .....</b>	<b>64</b>
6.3.1	Order information .....	64
6.3.2	Consumables and other parts order information .....	64
6.3.3	Basic package content .....	64
<b>6.4</b>	<b>Disposal Information .....</b>	<b>65</b>
6.4.1	Battery disposal .....	65
6.4.2	Disposal of patient-related accessories .....	65
6.4.3	Disposal at the end of its useful life .....	65
<b>6.5</b>	<b>Errors and Troubleshooting .....</b>	<b>66</b>
6.5.1	Error messages .....	66
6.5.2	General errors and troubleshooting .....	67
<b>6.6</b>	<b>Electromagnetic Interference .....</b>	<b>69</b>
6.6.1	Measures to prevent electromagnetic interferences .....	69
6.6.2	Additional measures .....	70
<b>7</b>	<b>Technical Data .....</b>	<b>71</b>
7.1	System Specifications .....	71
7.2	Classification and Safety Standards .....	73
7.3	Defibrillation Pulse .....	74
7.4	Shock Advisory System (SAS) .....	77
7.5	Configuration Settings .....	81
7.6	Telecommunication (options) .....	81
7.7	Electromagnetic Interferences .....	82
7.7.1	Electromagnetic emissions .....	82
7.7.2	Electromagnetic immunity .....	82
7.7.3	Recommended minimum distances .....	84
7.8	Literature .....	85
7.9	Glossary .....	85
7.10	Inspection Report .....	86
<b>8</b>	<b>Index .....</b>	<b>88</b>
<b>9</b>	<b>Appendix - Symbols .....</b>	<b>89</b>



# 1 Safety Notes

## 1.1 User Profiles

The following persons may use the **FRED PA-1**:

- **ACLS** Qualified medical personnel trained for Advanced Cardiac Life Support (ACLS), trained on the use of the **FRED PA-1**, may use the Automated External Defibrillator (AED) operating modes of the **FRED PA-1**.
- **BLS** Qualified medical personnel trained for Basic Life Support (BLS), semi-automatic defibrillation and Cardiopulmonary Resuscitation (CPR) on the **FRED PA-1** may use the AED operating mode of the **FRED PA-1** in semi-automatic or fully automatic mode.
- **Laypersons** People not trained in early defibrillation, as long as they can understand and follow spoken and illustrated instructions. The device can be used without any training, just by following the pictures and spoken instructions. Nevertheless, training to CPR is recommended to guarantee an optimal resuscitation procedure.



Laypersons must contact healthcare professionals (such as emergency services) immediately when they start to use the **FRED PA-1**.

## 1.2 Intended Use

### 1.2.1 General intended purpose

The **FRED PA-1** is intended for cardiac arrest management:

- Defibrillation (automatic, semi-automatic) of patients
- Provide heart massage (CPR) guidance.

#### Target population

The **FRED PA-1** can be used on any type of person either adults, children or infants with the appropriate electrode type (see the recommendations below).

		Type of electrode to be preferred	Alternative electrode that can be used
ADULT	Adult + paediatrics ≥ 8 years (or ≥ 25kg)	Adult electrodes	Adult electrodes
CHILD	Paediatrics ≥ 1 year and < 8 years (or < 25kg)	Child electrodes	Adult electrodes or Adult electrodes + Child adapter
INFANT	Paediatrics < 1 year	/	Child electrodes

#### Use environment

The portable **FRED PA-1** is intended to be used in the following environments:

- Pre-hospital care (excluding patient transportation)
- Patient's homes
- Public
- Workplaces

## 1.2.2 General warnings and precautions for use

### Responsibility of the user

- Regulations on who is allowed to use devices like the **FRED PA-1** and which training is required are country-specific. Legal regulations must always be observed.
- Before using the device, a SCHILLER representative must perform a presentation on the device's operation and safety measures if the local regulations require it.
- The numerical and graphical results and any interpretation given must be examined with respect to the overall clinical condition of the patient and the general recorded data quality.
- Damaged or missing components must be replaced immediately.
- The **FRED PA-1** must be stored in a place inaccessible to children and infants.
- Properly dispose of the packaging material and make sure it is out of reach for children and infants.
- The **FRED PA-1** is an emergency device and must be ready for operation at any time and in all situations.

### Check that:

- A set of adult electrodes is pre-connected, and a spare set of electrodes and/or a child adapter can be stored with the device.
- The **FRED PA-1** is always equipped with a sufficiently charged battery
- Always keep a new spare battery on hand
- An empty battery must not be reused and must be disposed of immediately
- If any serious incident has occurred in relation to the **FRED PA-1**, it should be reported to the manufacturer and the competent authority of the Member State in which the user or patient is established.
- A child adapter is available and attached to the handle of the **FRED PA-1**.

### Organisational measures

- Before using the **FRED PA-1**, ensure that an introduction regarding the **FRED PA-1** functions and the safety precautions has been provided and understood.
- Keep these operating instructions in an accessible place for reference when required. Check that they are always complete and legible.

### Safety conscious operation

- **Danger of electric shock.** Danger for the user, rescuer, and patient. The energy applied to the patient can be conducted through the patient to other persons, who may suffer a lethal electric shock. Therefore:
  - Do not touch the patient, the electrodes, the child adapter or other conducting objects during defibrillation.
  - Do not defibrillate the patient in a puddle of water or on other conducting surfaces.
  - Switch the **FRED PA-1** off when it is no longer used.
- **Danger of explosion.** The **FRED PA-1** must not be used in areas where there is any danger of explosion. There might be a danger of explosion in areas where flammable products (petrol), flammable anaesthetic agents or products for skin cleaning/disinfection are in use or where the ambient air's oxygen concentration is higher than 25%.
- Immediately report any changes that impair safety (including operating behaviour) to the responsible person.
- Only use original SCHILLER electrodes, accessories and supplies.
- Check that the **FRED PA-1**'s casing, electrode connections (and child adapter if applicable) are not damaged.
- Check the expiration date of the defibrillation electrodes on the packaging.

- After use; refer to Chapter [6 Maintenance](#)
- Immediately replace a damaged **FRED PA-1** or damaged cables, connections (and child adapter if applicable).
  - If the child adapter was present/installed and is now missing, replace it/provide a new one
- Operating the **FRED PA-1** with a defective casing, damaged cables constitutes or damaged child adapter (if applicable) a danger to life.
- Only operate the **FRED PA-1** in accordance with the specified technical data. Refer to chapter [7 Technical Data](#)
- Do not operate the **FRED PA-1** in any moving vehicle.

### 1.2.3 Defibrillation function

#### Intended purpose

The **FRED PA-1** is intended for defibrillation (AED). It also provides CPR feedback (guidance to heart massage).

- The device software determines if an electric shock is required based on the analysis of the heart rhythm.
- If a shock is needed, the device delivers automatically (automatic version) or prompts the user to press the shock button to deliver the shock (semi-automatic version).
- The device also provides advice to perform heart massage (CPR). Several options are possible for CPR guidance:
  - A metronome prompts a regular sound to indicate the adequate rate for chest compressions.
  - The FreeCPR option provides real time feedback on the chest compressions and support the user to adapt its heart massage frequency.
  - The **FRED PA-1** online version uses the 4G network for intervention data transmission and maintenance management of devices (alerts).

## 1.3 Medical Indications



- ▲ The defibrillator is intended to be used on the patient in suspected cardiac arrest (no normal breathing, no conscious reaction). The defibrillator software can decide to deliver an electrical shock or to guide the user to perform proper heart massage (CPR) depending on the heart rate analysis.

## 1.4 Clinical Benefits



- ▲ The benefit of the application of a defibrillator is to diagnose and treat a patient in cardiac arrest, expecting an increase of his chances of survival.
  - Overall survival to cardiac arrest is known to be dismal (usually lower than 10%). Nevertheless, depending on the efficiency of the rescue chain, including public access lay responders, survival can reach more than 50% for patients that are early shocked after collapse (Valenzuela et al. 2000) + (Bækgaard et al. 2017).
- ▲ Survival depends on restoration of an organised rhythm and a spontaneous circulation, which derives from the following performances: diagnostic of the cardiac rhythm, defibrillation efficiency, and efficiency of the bundle of care applied to the patient. Thus, the clinical benefit can be assessed through the measurement of clinical performances.

## 1.5 Contraindication for Use



### AED mode


- ▲ The defibrillator must not be used when the person:
  - Is responsive
  - Is breathing normally

### Other contraindications

- ▲ Do not use the **FRED PA-1** in or near Magnetic Resonance Imaging (MRI) equipment.
- ▲ **Danger of explosion.** The **FRED PA-1** must not be used in areas where there is any danger of explosion (high oxygen level, flammable products, etc).
- ▲ The **FRED PA-1** is not intended to be used in any moving vehicle.
- ▲ The **FRED PA-1** is not designed for sterile use.

## 1.6 Operation with other Devices



- ▲ Magnetic and electrical fields from x-ray or tomographic devices, portable radio equipment, HF radios and devices labelled with the  symbol can affect the operation of this device (refer to section [7.7 Electromagnetic Interferences](#)). Avoid using such devices or keep a sufficient distance from them.
- ▲ **FRED PA-1** is not intended to be operated while using high-frequency surgical devices.
- ▲ **Interference with other devices.** The charging of energy and the release of the defibrillation impulse can disturb other devices. Check these devices before their further use.
- ▲ Other medical equipment applied to a patient which has no defibrillation proof applied part must be disconnected from the patient.
- ▲ The patient can be endangered by too high leakage currents (summation of leakage currents) if several devices are connected to the patient. For this reason, devices that are not required should be disconnected from the patient, and only equipment approved by SCHILLER may be connected to the **FRED PA-1**.
- ▲ If the patient has a pacemaker implanted, do not position the electrode directly onto the pacemaker. Check the pacemaker after the defibrillation.

## 1.7 Maintenance and Cleaning



- ▲ **Danger of electric shock.** Do not open the **FRED PA-1**. There are no serviceable parts inside. Refer servicing to qualified personnel only.
- ▲ Do not service, maintain or clean the **FRED PA-1** while in use with a patient.
- ▲ Before cleaning, switch the **FRED PA-1** off and remove the battery.
- ▲ Do not use high-temperature sterilisation processes (such as autoclaving). Do not use E-beam or gamma radiation sterilisation.
- ▲ Do not use aggressive or abrasive cleaners (refer to section [6.2 Cleaning and Disinfecting](#)).
- ▲ Do not, under any circumstances, immerse the **FRED PA-1** or cable assemblies in liquid.
- ▲ To ensure patient safety, only use original SCHILLER accessories. The user is responsible for the use of third-party accessories. The warranty does not cover damage resulting from the use of accessories or consumables other than those marketed by SCHILLER.

## 1.8 Known Side Effects



- Defibrillating a patient can cause:
  - Skin irritations or burns
  - Malfunction or damage of implanted pacemaker

## 1.9 General Notes for FRED PA-1



A defibrillation can fail with certain disease patterns.

## 1.10 Cybersecurity

### 1.10.1 Networks and internet



- ▲ The security of the network is the sole responsibility of the user.
- ▲ When the **FRED PA-1** is part of a network (LAN, WLAN, HIS) or any other transmission/reception medium, or if exposed to the Internet or other insecure networks, appropriate security measures must be taken to protect the stored patient data.
- ▲ To guarantee the cybersecurity of the network, SCHILLER recommends the following:
  - Isolating the **FRED PA-1** network from other networks
  - Defining access authorisation for the configuration of the host system, including the **FRED PA-1**, so that no unauthorised alterations of the system are possible.
  - Use Transport Layer Security (TLS) 1.2 or higher for communication with system server and SDM server.
- ▲ If the connection between the **FRED PA-1** and the server is bad or loss, this can result in an impossible analysis of post-intervention data. The user should identify, analyse, evaluate, and control these risks related to the connection to networks.
- ▲ Any changes to the networks could introduce new risks that require additional analysis by the user. These changes include:
  - Changes in network configuration
  - Connection/disconnection of (additional) items
  - Update/upgrade of the **FRED PA-1**

### 1.10.2 Patient data (personal data)



- ▲ Patient data security is the sole responsibility of the user. Therefore:
  - Delete personal data (intervention file) before sending the device for repair or maintenance.
  - If the device has been sent to SCHILLER with personal data, the data is deleted before starting the repair or maintenance process.

#### Exception investigation in case of incident reporting

- ▲ If the **FRED PA-1** is sent for investigation in case of incident reporting, the intervention data are very important to detect the cause. Therefore:
  - The **FRED PA-1** can be sent to SCHILLER by the responsible organisation with personal data
  - The intervention file with the personal data can be exported if possible (refer to section [5.1.1 For standard FRED PA-1 with an SD card](#)) and sent to SCHILLER by the responsible organisation.
  - After the investigation, SCHILLER confirms that all personal data has been deleted from services, applications, and the **FRED PA-1**. The **FRED PA-1** is returned to the customer without any personal data.

### 1.10.3 Setup security guidance



- ▲ For the online version prefer network communication rather than an SD card for updates
- ▲ Do not use self-signed certificate on the server.
- ▲ For networks and the internet; refer to section [1.10.1 Networks and internet](#)

## 1.11 Additional Terms

### 1.11.1 Implied authorisation

Possession or purchase of the **FRED PA-1** does not convey any express or implied license to use the **FRED PA-1** with replacement parts which would alone, or in combination with the **FRED PA-1**, fall within the scope of one or more patents relating to the **FRED PA-1**.

### 1.11.2 Terms of warranty

Your SCHILLER **FRED PA-1** is warranted against defects in material and manufacture according to the general terms of condition. Excluded from this warranty is damage caused by an accident or as a result of improper handling. The warranty entitles to free replacement of the defective part. Any liability for subsequent damage is excluded. The warranty is void if unauthorised or unqualified persons attempt to make repairs.

In case of a defect, send the **FRED PA-1** to your dealer or directly to the manufacturer. The manufacturer can only be held responsible for the safety, reliability, and performance of the apparatus and honour the warranty, if:

- Persons authorised by him are permitted to carry out assembly operations, extensions, readjustments, modifications, or repairs,
- Spare parts used for assembly operations, extensions, readjustments, modifications or repairs are recommended or supplied by SCHILLER.
- The SCHILLER **FRED PA-1** and approved attached equipment are used in accordance with the manufacturer's instructions.



There are no express or implied warranties which extend beyond the warranties herein/above set forth. SCHILLER makes no warranty of merchantability or fitness for a particular purpose with respect to the product or parts thereof.

#### **Support period**

Software updates are available for 10 years from the date the last **FRED PA-1** was placed on the market.

### 1.11.3 Reporting security incidents and vulnerability disclosure policy

If you think you have found a vulnerability in one of our products or services, send us the details to [customercomplaint@schiller.fr](mailto:customercomplaint@schiller.fr). SCHILLER will acknowledge your message within 3 days and verify the reported vulnerability within 10 days. Allow 90 days before disclosing this/any vulnerability publicly.

## 1.12 Symbols and Indicators

### 1.12.1 Symbols used in this user guide

The safety levels are classified according to ANSI Z535.6. The following overview shows the safety symbols and pictograms used in this user guide. Danger, Warning, and Caution are used in this user guide to point out potential dangers and indicate risk levels. Familiarise yourself with their definitions and significance.



This symbol warns of possible direct danger, which could lead to severe personal injury or death.



This symbol warns of a possible dangerous situation that could lead to severe personal injury or death.



This symbol warns of a dangerous situation that could lead to personal injury and/or indicate possible property damage.



For general safety notes as listed in this section.



For electrical hazards, warnings or precautionary measures when dealing with electricity.



This symbol warns of dangerous situations that could damage property or system failure and provides other important user information.

### 1.12.2 Symbols used on the FRED PA-1

For generally used symbols; refer to Chapter [13 Appendix - Symbols](#)



BF symbol. The **FRED PA-1** signal input is defibrillation-protected. Type BF Applied parts



Dangerous voltage. Used for electrical dangers during defibrillation.



Symbol for the identification of electrical and electronic equipment.

- The **FRED PA-1** must be disposed of in a municipally approved collection point or recycling centre when it is no longer required.
- Improper disposal harms the environment and human health due to the presence of dangerous substances in electrical and electronic equipment.



Read the instructions for use

**IP55**

The **FRED PA-1** is protected against dust and spraying water from all directions.



#### Devices with a cellular connection

Attention. Non-ionising electromagnetic radiation. The **FRED PA-1** contains an HF transmitter.

The **FRED PA-1** radiates high-frequency electromagnetic energy during telemetric ECG data transfer and can disturb other devices if not installed and operated in accordance with the user guide.

However, even in the case of correct installation/operation, there is no guarantee that no interferences can occur.

If the **FRED PA-1** causes interferences, these can be prevented by switching it off.

The user can take the following measures to solve this problem:

- Increase the distance between the disturbed device and the **FRED PA-1**. A minimum distance of 20 cm must be kept between the **FRED PA-1** and a pace-maker.
- Turn the **FRED PA-1** to change the antenna's angle of radiation.

For more details; refer to section [6.6 Electromagnetic Interference](#).



The **FRED PA-1** cover features the sign designed by ILCOR to locate and identify an AED (Automated External heart Defibrillator).



Maintenance required



Language selection / repeat button















Emergency phone




Recyclable / renewable plastic

**1.12.3 Symbols used on the batteries**

	The unit/component can be recycled
 MM/YY	Primary Lithium Manganese dioxide (Li-MnO <sub>2</sub> ) battery, do not charge.
	Do not short-circuit
	Do not dispose in fire / Do not incinerate
	Do not open or dismantle
	Do not deform or damage
	Minimum/maximum discharging temperature for Lithium/MnO <sub>2</sub> battery
	Note: Storage at maximal discharging temperature increases the self-discharge of the battery.
	Batteries must not be disposed of with domestic refuse
	Read the instruction for use
 YYYY-MM	Expiry date of the primary Li-MnO <sub>2</sub> battery
	Direct current
	Positioning of primary battery


### 1.12.4 Symbols used on the electrode packaging

For generally used symbols; refer to Chapter 13 Appendix - Symbols

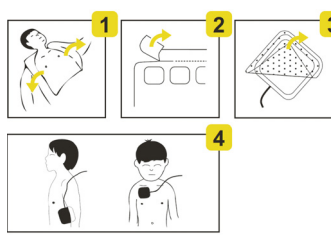

#### PAEDIATRIC

1. Remove the clothing from the patient's chest
2. Open pouch beginning at the notch
3. Remove protecting film from electrodes
4. Antero-Lateral electrode placement for children

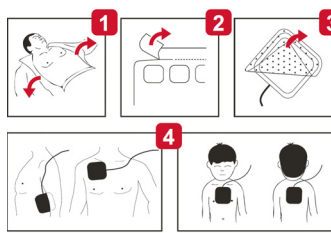

#### ADULT

1. Remove the clothing from the patient's chest
2. Open pouch beginning at the notch
3. Remove protecting film from electrodes
4. Antero-Lateral and Antero-Posterior electrode placement




Do not reuse



Do not bend packaging



Do not use if packaging is damaged



Storage temperature for the electrodes



Expiry date of the electrodes



An open package cannot be conserved for more than one day.



Keep away from sunlight



Keep dry



Do not use more than 24 hours



For use by or on the order of a physician or person licensed by state law



Reading this user guide is mandatory before using the electrodes.



Recyclable/renewable - Low-density polyethylene - Plastic/aluminium (composite material)



Device is equipped with Radio Frequency Identification RFID tag



The product is intended for use for adults (>25kg)



The product is intended for use for children (<25kg)

### 1.12.5 Symbols specific to the child adapter

For generally used symbols; refer to Chapter [13 Appendix - Symbols](#)



Read the instruction for use



Symbol for the recognition of electrical and electronic equipment.

- The child adapter must be disposed of in a municipally approved collection point or recycling center when it is no longer required.
- Improper disposal harms the environment and human health due to the presence of dangerous substances in electrical and electronic equipment.



Dangerous voltage. Used for electrical dangers during defibrillation.



Child only. The product is intended for use on patients weighing less than 25 kg.



Manufacturer information



Manufacturing date



Reference number



Batch code



CE marking, affirms its conformity with European standards



Warning

## 2 Components and Operation

### 2.1 General Information

**FRED PA-1** is an AED. The **FRED PA-1** is available as an automatic and semi-automatic defibrillator.



Local laws and regulations regarding the use of an AED vary from country to country. While some countries allow laypersons to use AEDs without any special training, other countries restrict the use of AEDs to Emergency Medical Technicians or First Responders after they have undergone special training.



#### **Biocompatibility**

The parts of the **FRED PA-1** described in this user guide, including all accessories that come in contact with the patient during the intended use, fulfil the biocompatibility requirements of the applicable standards. If you have any questions in this matter, contact SCHILLER.

## 2.2 Design

### 2.2.1 General design

**Defibrillator** **FRED PA-1** is a defibrillator featuring the BTE (biphasic truncated exponential) waveform. The patient receives a defibrillation shock using disposable electrodes. The ECG signal is analysed using the same electrodes; in addition, the user is guided by voice prompts and pictograms (loudspeakers/LEDs next to pictograms). The **FRED PA-1** recognises the connected electrodes and selects the defibrillation energy accordingly:

- Adult electrode
- Adult electrode via child adapter
- Child electrode

An RFID tag in the connector (for electrodes with article no. 0-21-0040) allows checking the shelf life of the electrodes when connected to the **FRED PA-1**.

**Languages** The **FRED PA-1** can be provided with different languages. Optional configuration with 3 languages, selectable after switching the **FRED PA-1** on.

**Metronome** The **FRED PA-1** emits a sound pace for CPR. The CPR rate is configurable.

**FreeCPR (option)** A CPR Guide with FreeCPR based on the impedance measurement by the defibrillation electrodes.

**Data memory** The **FRED PA-1** is equipped with an internal memory. During the intervention, data can, therefore, be saved, including the analysed ECG data. In addition, technical data (logs) are stored.

**Data transmission** The **FRED PA-1** has an SD card slot in order to:

- Retrieve data via an SD card
- Perform software and configuration updates

The **FRED PA-1** online version has a cellular network connection to connect to the LifeDataNet G2 Server for device pool management and intervention data transmission.

**Power supply (standard)** The **FRED PA-1** is operated with a non-rechargeable, disposable lithium battery. The battery capacity is sufficient for (if the **FRED PA-1** is stored/used in optimal temperature conditions between 15 to 25°C):

- More than 140 shocks at maximum energy
- 4 hours and 30 minutes of continuous operation with intermittent charging.

#### **For devices with an SD card**

- Several years in standby. Standby duration corresponding to laboratory tests at 25°C, 6 years with weekly self-tests.

#### **For devices with cellular network**

- Several years in standby. Standby duration corresponding to laboratory tests at 25°C, with a constant, good GSM connection and without antenna roaming, 3 years with weekly self-tests.

#### **Self-test**

To ensure its readiness for use, the **FRED PA-1** performs a daily or a weekly self-test (refer to section [6.1 Maintenance Intervals](#)). Self-test includes a test of the charging circuit and battery capacity. If this test is completed successfully, the green Ready-To-Use (RTU) LED blinks (at two-second intervals), showing that the **FRED PA-1** has not detected an error.

**Cellular network (option)** The **FRED PA-1** equipped with a cellular network is connected to the LifeDataNet G2 Server for device pool management and intervention data transmission.

### 2.2.2 Available versions

Model	Description
FRED PA-1 Semi-automatic	AED Semi-automatic
FRED PA-1 Automatic	AED Fully automatic
FRED PA-1 Semi-automatic Online	AED Semi-automatic with 4G connection
FRED PA-1 Automatic Online	AED Fully automatic with 4G connection

## 2.3 Operating and Display Elements

### 2.3.1 FRED PA-1 overview




2.3.2 Operating elements

In addition to the voice prompts, the resuscitation steps are indicated by pictograms and the current step is highlighted with a flashing LED.


**FRED PA-1 with one language**

As soon as the cover of the **FRED PA-1** is opened, the **FRED PA-1** starts issuing audio prompts. The last message is repeated when the **Repeat** button is pressed.

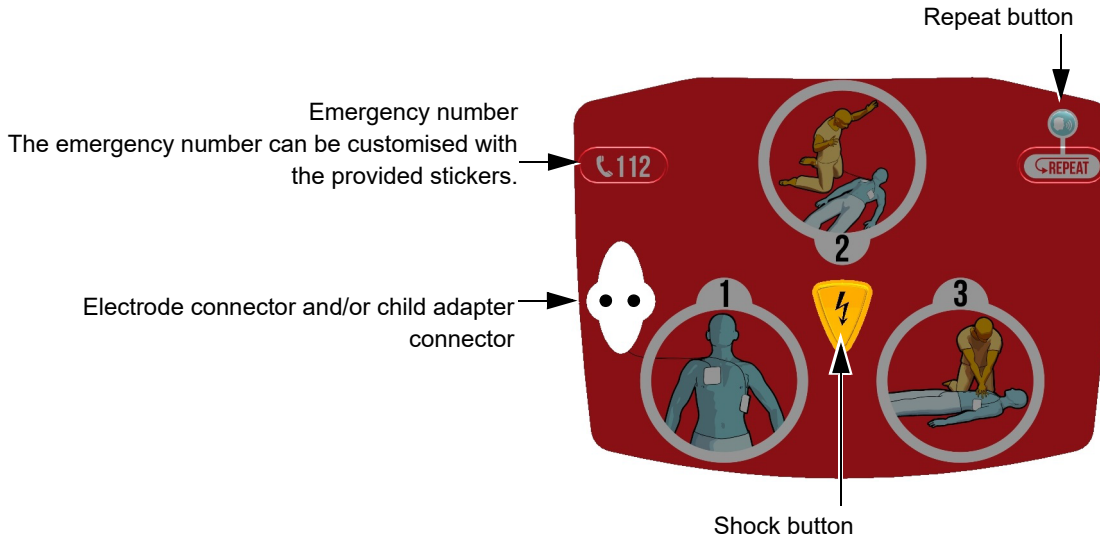

**Multiple language FRED PA-1**

As soon as the cover of the **FRED PA-1** is opened, the **FRED PA-1** starts issuing audio prompts in the default language. The two other languages can be selected at any time during the resuscitation procedure by pressing the button above the flag label.

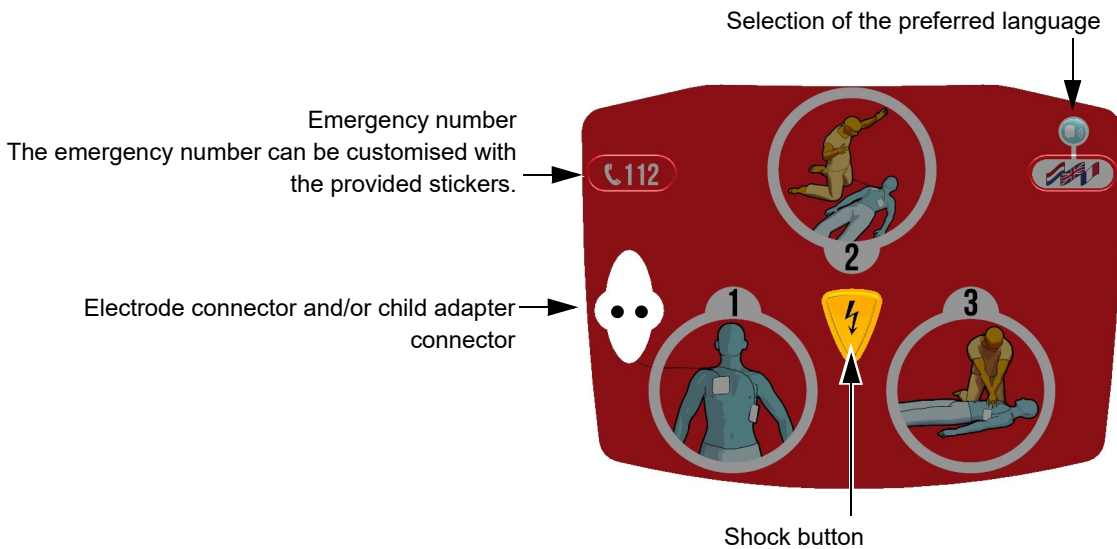

## 2.4 Function

### 2.4.1 Automatic self-test

Self-test includes the test of the charging circuit and the battery capacity.

#### Battery insertion

Immediately after a battery has been inserted, the **FRED PA-1** performs a test of the components and battery. If this test is completed successfully, the RTU LED is blinking and all service status LEDs are off, showing that the **FRED PA-1** has not detected an error.

#### RTU Test

To ensure its readiness for use, the **FRED PA-1** performs a daily or weekly self-test at 12:00 AM. This setting must only be configured by service personnel authorised by SCHILLER (refer to section [6.1 Maintenance Intervals](#)).

If a problem is detected during this test:

- An acoustic alarm is issued,
- The RTU LED stops blinking
- The service LEDs give additional information.



Fig. 2.1 LED indicator



#### Additional information

- If an alarm is in progress (visual and acoustic), the battery autonomy is reduced.
- In addition, the device performs a daily or weekly self-test (this setting must only be configured by service personnel authorised by SCHILLER)
- An alarm (visual and acoustic) can only be reset by removing and reinserting the battery.
- For the alarm details; refer to section [6.5.1 Error messages](#).

## 2.4.2 Defibrillation procedure

The user is guided through all operation steps by verbal instructions and the pictogram on the **FRED PA-1**. When the **FRED PA-1** is ready for shock delivery, the user is advised not to touch the patient, and a warning tone with the illuminated high voltage symbol is activated.

### **The FRED PA-1 runs in semi-automatic mode**

This means that the user must release the shock. When the **FRED PA-1** is switched on, the user is prompted to apply the electrodes to the patient. Next, they are prompted not to touch the patient during the analysis phase. For the duration of the analysis; refer to section [7.4 Shock Advisory System \(SAS\)](#). Depending on the result, the user is prompted to deliver a shock or to start with CPR.

### **The FRED PA-1 runs in automatic mode**

The **FRED PA-1** delivers defibrillation shocks automatically; that is, there is no need to trigger the shock. When the **FRED PA-1** is switched on, the user is prompted to apply the electrodes to the patient. Next, they are prompted not to touch the patient during the analysis phase. For the duration of the analysis; refer to section [7.4 Shock Advisory System \(SAS\)](#). If a shock is advised, a countdown accompanies the last 3 seconds before the shock is automatically delivered.

## 3 Initial Operation

### 3.1 General Information and Safety Notes



#### Danger of explosion

- ▲ The **FRED PA-1** must not be used in areas where there is any danger of explosion. Areas may be susceptible to explosion if flammable substances (gas), flammable anaesthetics, or products used to clean or disinfect the skin are used. Moreover, the defibrillator must not be used in an environment that is favourable to combustion. This is the case when ambient air contains more than 25% oxygen or nitrous oxide (laughing gas). Oxygenation in the vicinity of the defibrillation pads must be strictly avoided. Less than 25% oxygen in the ambient air is considered safe. Dangerously high oxygen concentrations can only occur in oxygen masks or enclosed areas, such as hyperbaric chambers.



#### Danger of explosion

- ▲ The battery must not be exposed to high-temperatures or disposed of with household waste.
- ▲ Do not expose the battery to chemicals that could dissolve ABS, polypropylene, polyvinyl chloride, nickel, mylar or steel.
- ▲ Do not short-circuit, cut, destroy, burn or charge (Li/MnO<sub>2</sub> battery) a battery.
- ▲ Always use the protective cover when storing spare batteries.

#### Patient hazard incorrect battery capacity indication

- ▲ A new battery is initialised when first inserted
- ▲ Replace the battery if the **FRED PA-1** indicates a battery problem. A defective battery must not be used.
- ▲ Turn off the **FRED PA-1** before removing the battery.



#### Patient hazard ensuring operational readiness

- ▲ Check that the **FRED PA-1** is always equipped with a sufficiently charged battery.
- ▲ The expiration date of a new battery, stored in its original packaging at a temperature of 25°C, is indicated on its packaging. It must not be used beyond this date.
- ▲ The protective cap of the battery must remain on during the entire storage time. The protective cap must only be removed when the battery is used.
- ▲ Do not expose the **FRED PA-1** to direct sunlight or to extreme hot or cold. An ambient temperature higher than 25°C has an adverse effect on the battery life.



Each time the **FRED PA-1** is turned on, it checks that the battery is functioning properly.

### 3.2 Inserting the Battery

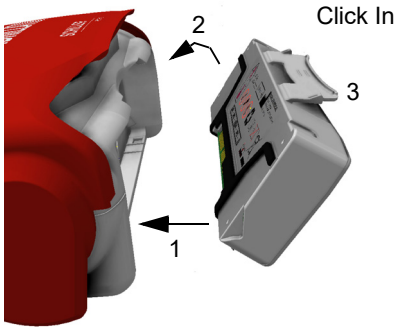


Fig. 3.1 Inserting the battery

Insert the battery as indicated in the illustration on the left.

1. Insert the two stop blocks located at the bottom of the battery in the **FRED PA-1** slots.
2. Perform a rotational movement until the battery locks in place.
3. As soon as the battery is inserted, the **FRED PA-1** runs a self-test to check the condition of the **FRED PA-1** and the battery.

During the test, the modem LED is on, and the electrode LED is blinking. This test can last for more than 1 minute.


If this test does not reveal any problems, the RTU is blinking, and all service status LEDs are off, showing that the **FRED PA-1** has not detected an error.



If the **FRED PA-1** is used on a patient, this test can be cancelled by opening the cover.

### 3.3 Adding Emergency Number Stickers


If your country's emergency number differs, apply the sticker with the correct one.

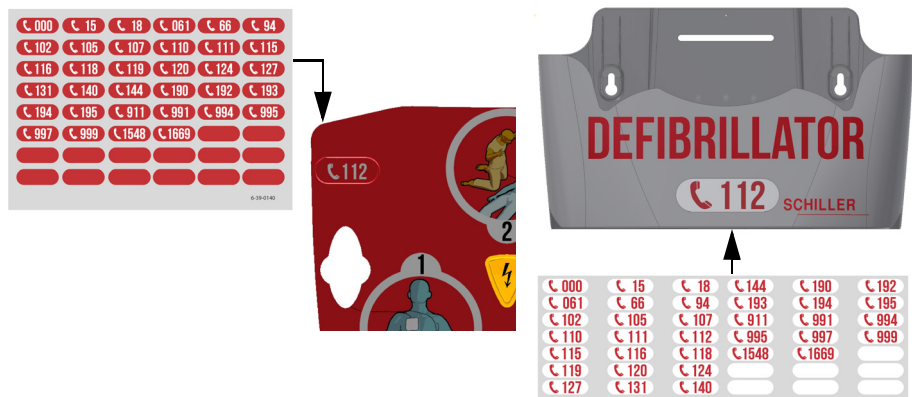

### 3.4 Attach the child adapter (if applicable)

Attach the child adapter as indicated in the illustration on the bottom.

1. Pass the strap around the handle.

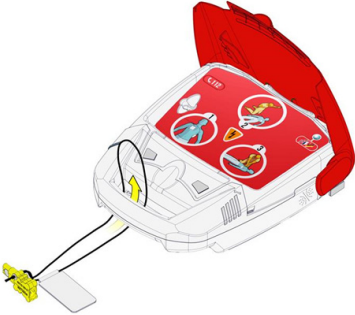


2. Slide the child adapter into the loop.



3. Store the child adapter under the cover.

After the installation:

- Check if the strap is long enough to be inserted into the FRED PA-1 connector.
- Check that the magnet is present at the back of the child adapter.

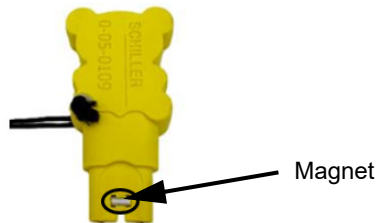

4. Close the cover.



### 3.5 Switching the FRED PA-1 On/Off

- Switching ON** → Open the cover. The 3 LEDs for the resuscitation steps are briefly lit.
- Switching OFF** → Close the cover.



**Forced shutdown procedure**

If the **FRED PA-1** cannot be switched off normally (closing the cover), remove the battery and reinsert it after 10 seconds.



- ▲ If a patient is detected while closing the cover, the **FRED PA-1** remains on, and the resuscitation process goes on.



If the cover is re-opened within 30 seconds after closing, the device resumes the intervention.

## 3.6 Battery Monitoring



- The lithium battery ensures that the **FRED PA-1** stays fully operative (and performs the self-test) for several years (at a temperature between 15 to 25°C), provided that the **FRED PA-1** is not being used.
- Battery service life depends on **FRED PA-1** use and ambient conditions.
- The battery must be replaced once the expiration date has been exceeded.
- The old battery must be recycled in accordance with local regulations.

### 3.6.1 Sufficient battery capacity



The RTU LED (green) on the **FRED PA-1** is blinking when the battery capacity is sufficient to perform the resuscitation protocol.

### 3.6.2 Low battery capacity indication



- Low battery capacity indication is the same during self-test, after the battery has been inserted, and during use.
- Despite the low battery indication, the **FRED PA-1** can still be used as normal and is still able to defibrillate.
- Always switch off the **FRED PA-1** before removing the battery.
- The remaining battery capacity depends on the use and ambient conditions.



Fig. 3.2 Low battery indication

If the battery capacity falls below 10%, the RTU LED (1) and the orange battery LED (2) are blinking. These indications are issued until the battery is replaced. The battery must be replaced as soon as possible.

### 3.6.3 Battery depleted during use, limited mode CPR



**Patient hazard**


▲ Defibrillation is no longer possible if a depleted battery is detected. The battery needs to be replaced immediately.

**Depleted battery while in use**

The **FRED PA-1** prompts the user to replace the battery and perform CPR. An audible signal is emitted. The RTU LED is off, and the orange battery LED blinks until the battery is replaced.

**Depleted battery during self-test**

An audible signal is emitted, the main status LED (1) is off, and the battery LED (2) blinks until the battery is replaced.

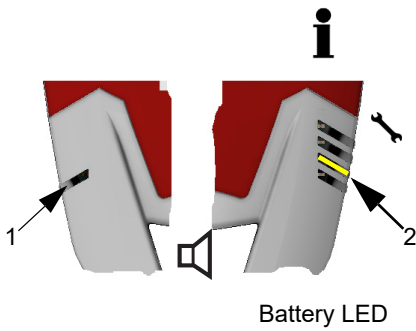

## 3.7 Replacing the pre-connected Pads and child adapter


### 3.7.1 Expired pads

The **FRED PA-1** is delivered with pre-connected pads. To replace the pads after use or if their shelf life has expired, proceed according to the following instructions:



- Only use the pads up to their expiration date.
- Note that the expiration date of the pads only applies if the vacuum pack is intact.
- Do not reuse the pads.

### 3.7.2 Connect the electrodes

1. Remove the battery
2. Remove the sticker with the LOT/Expiration date  from the electrode pouch and stick it above the RTU LED (1).
3. Open the cover
4. Connect the electrode cable to the **FRED PA-1** (2)
5. Put the electrode pack in the cover and close the cover.
6. Check that the cover does not squeeze/compress the electrode cable or the electrode packaging when closed.
7. Insert the battery.
8. The **FRED PA-1** is ready for use when the RTU LED is blinking, and the service LEDs are off.
9. If requested, add a spare set of electrodes in the compartment on the **FRED PA-1** underside.




### 3.7.3 Child adapter



1. Remove the protecting packaging of the child adapter and attach the strap to the **FRED PA-1** handle.  
[3.4 Attach the child adapter \(if applicable\)](#)
2. Then carefully lay the adapter on the red folio and close the cover.

### 3.7.4 Connect the electrodes with the child adapter

1. Remove the battery
2. Remove the sticker with the LOT/Expiration date  from the electrode pouch and stick it above the RTU LED (1).
3. Open the cover
4. Connect the electrode cable to the FRED PA-1 (2)
5. Slide the electrode pack in the cover and close the cover.
6. Check that the cover does not squeeze/compress the electrode cable or the electrode packaging when closed.
7. Insert the battery after closing the cover.
8. The **FRED PA-1** is ready for use when the RTU LED is blinking, and the service LEDs are off.
9. If requested, add a spare set of electrodes in the compartment on the **FRED PA-1** underside

# 4 Defibrillation

## 4.1 Instructions and Safety Notes

### 4.1.1 Instructions



- AHA and ERC's last guidelines for ALS recommend that when treating an adult with a permanent pacemaker or an ICD, the defibrillator external pads should be placed on the chest wall, ideally at least 8 cm from the generator position. Moreover, the antero-lateral and antero-posterior pad placements on the chest are acceptable in patients with a permanent pacemaker or ICD. After restoration of spontaneous circulation, the pacemaker should always be checked for possible damage.
- The **FRED PA-1** is a high-voltage electrotherapy device. Only personnel authorised by local law are permitted to use these devices. Improper operation can endanger life.
- Non-medical personnel are only permitted to use an AED such as the **FRED PA-1** if local law approves of this practice.
- The success of the defibrillation depends not only on the correct application of the defibrillator but also on the heart's condition. It is the physician's responsibility to take any additional measures (for example, adrenaline).
- According to the AHA/ERC guidelines, even children and infants (under 8 years) may be defibrillated.
- The adult electrodes should be applied in the antero-lateral position when used on adult patients (older than 8 years or weighing more than 25 kg).
  - With children weighing less than 25 kg or who are younger than 8 years old, it is recommended to apply the adult electrodes (surface area 80 cm<sup>2</sup>) antero-posterior with child adapter.
  - The adult electrodes must be connected to the child connector and the latter must be then connected to the **FRED PA-1**.  
See chapter [4.2.1 General information](#)
- When defibrillating children with child electrodes (surface area 42 cm<sup>2</sup>), it is recommended to choose the antero-lateral position.
- When defibrillating infants with child electrodes (surface area 42 cm<sup>2</sup>), it is recommended to choose the antero-posterior position.
- For defibrillation of infants (< 1 year old), follow the local guidelines.
- A defibrillation can fail with certain disease patterns.

#### Patients with implanted pacemakers

- **FRED PA-1** features an electronic pacer pulse suppression algorithm, and therefore, pacemaker pulses are not considered during the analysis. Depending on the pacemaker model and the position of the electrodes, the compensation pulse following every pacer pulse may be considered as a QRS complex. In this case, the analysis can be distorted and inaccurate. It depends on the pacer pulse parameters whether or not the compensation pulse is counted as a QRS complex.
- The required energy for a successful defibrillation depends on several parameters (Body composition). For emergency medical treatment, AHA/ERC recommend a biphasic impulse. Depending on configuration settings, the energy of the first three shocks can be increased.

### 4.1.2 Safety notes for defibrillation use



- ▲ Changes, including the operational behaviour, affecting safety must be immediately reported to the responsible.

#### Shock hazard for patients

- ▲ In unfavourable situations, the possibility of ECG analysis errors should not be dismissed. The **FRED PA-1** must, therefore, only be used if the following symptoms are found:
  - Not responsive
  - No respiration
  - No pulse



#### Shock hazard for users and assistants

- ▲ Position the patient flat on a firm, electrically insulated surface.
- ▲ Check that there are no conductive connections between the patient and other persons during ECG analysis and defibrillation.
- ▲ The patient must not come into contact with metal parts, a bed, or a stretcher in order to prevent secondary contacts or paths for the defibrillation current that could endanger the assistants. For the same reason, do not position the patient on a wet surface (rain, swimming pool accidents).
- ▲ The operator must avoid contact between parts of the patient's body, such as exposed skin of the head or limbs, conductive fluids such as gel, blood, or saline and metal objects such as a bed frame or a stretcher, which may provide unwanted pathways for the defibrillating current.
- ▲ Do not allow the defibrillation electrodes to come into contact with other electrodes or metal parts which are in contact with the patient.
- ▲ The patient's chest must be dry because moisture can cause unwanted pathways for the defibrillation current. For safety, wipe off flammable skin cleansing agents.
- ▲ The assistants' tasks must be clearly defined as follows:
  - During ECG analysis and shock:
    - Suspend CPR
    - Check that the patient lies as motionless as possible
    - Do not touch the patient; otherwise, artefacts may lead to incorrect analysis results, and the recommended shock is cancelled.
  - Immediately prior to the shock:
- ▲ Stop chest compressions and CPR

#### Risk of skin burns for the patient

- ▲ Due to the high currents, there is a risk of skin burns at the electrode application site. Therefore, the electrodes must not be placed on or above:
  - The sternum
  - The clavicle
  - The nipples
- ▲ Delivering defibrillation shock with bad contact or delivering repeated shock might lead to tissue redness or burns.
- ▲ Do not use expired electrodes.



**Risk of malfunction of implanted pacemaker**

- ▲ Defibrillating a patient with an implanted pacemaker is likely to impair the pacemaker function or cause damage to the pacemaker.

For this reason:

- Defibrillation pads must not be positioned near the pacemaker
- The pacemaker must be checked immediately after finishing the therapy.

**Risk of malfunction**

- ▲ Using a defibrillator in AED mode in a moving vehicle can interfere with SAS and lead to false decisions related to patient treatment advice.
- ▲ The agonal respiration phenomenon (GASP) of a patient in cardiac arrest may interrupt the analysis process.
- ▲ The presence of chest compressions during analysis may interrupt the ECG analysis.

4.1.3 Defibrillating child and infant patients



- ▲ For the defibrillation of child and infant patients, the child pads (yellow connector, see left) should be used.
- ▲ If no child pads are available, first use the adult electrodes connected to the child adapter. If no child pads and no child adapter are available, adult electrodes can be used for children as a last resort. In such case, the energy setting is not adapted.
  - The energy is set to child mode automatically when you connect the adult electrodes via the child adapter to the **FRED PA-1**.
  - Adult electrodes must be placed antero-posterior.
- ▲ When using an adult electrode without the child adapter, the energy setting is set to adult mode.
- ▲ Always use child pads or child adapter to defibrillate child and infant patients weighing less than 25 kg or younger than 8 years old while using the **FRED PA-1**.



Fig. 4.1 Child electrode

- In first instance, always use child pads to defibrillate child patients weighing less than 25 kg or younger than 8 years old while using the **FRED PA-1**.
  - If child pads are not available and if child adapter is available, use it with adult electrodes to defibrillate child patients weighing less than 25 kg or younger than 8 years old while using the **FRED PA-1**.
  - If neither child pads nor child adapter are available use adult pads.
- For infants, the preference is to use child pads.
  - Child pads can be recognised by specific package labeling of the electrodes and their yellow connector.
  - Child adapter Id pads can be recognised by specific package labeling (and tag) of the adapter and their yellow colour.
  - Adult pads Id pads can be recognised by specific package labeling of the electrodes and their blue connector.
- The child electrodes (surface area 42 cm<sup>2</sup>) should be applied in the **antero-lateral** position on children and antero-posterior on infants.
- When child pads are connected to the **FRED PA-1**, the energy setting is automatically adapted:
  - 1<sup>st</sup> shock: 50 joules
  - 2<sup>nd</sup> shock: 50 joules
  - 3<sup>rd</sup> shock: 50 joules
- If no child pad is available, you can use the adult pad connected via the child adapter.
- Apply the adult electrodes (surface area 80 cm<sup>2</sup>) **antero-posterior** position on the child.
- The energy setting is automatically adapted:
  - 1<sup>st</sup> shock: 50 joules
  - 2<sup>nd</sup> shock: 50 joules
  - 3<sup>rd</sup> shock: 50 joules



Fig. 4.2 Child adapter



**Fig. 4.3** Adult electrode

- If neither children pads nor child adapter are available, use adult pads to defibrillate child patients. Adult pads can be recognised thanks to the packaging of the electrodes and their blue connector.
- The adult electrodes (surface area 80 cm<sup>2</sup>) should be applied in the **antero-posterior** position.
- When adult pads are connected to the **FRED PA-1**, the energy setting is automatically adapted:
  - 1<sup>st</sup> shock: 150 joules
  - 2<sup>nd</sup> shock: 200 joules
  - 3<sup>rd</sup> shock: 200 joules

## 4.2 Application of the Adhesive Electrodes



- ▲ Do not reuse the pads. If reused, the electrical properties may be insufficient, which could lead to patient injury.




- ▲ Only use pads up to their expiration date. Note that the indicated expiration date only applies if the vacuum pack is intact.
- ▲ The pads are pre-gelled, so there is no need to use an extra contact agent.
- ▲ The placement of pads may be different depending if the patient is an adult, child or infant.

### 4.2.1 General information




The child adapter is stored in the defibrillator cover, attached to the handle of the **FRED PA-1** with a strap and can be accessed when the cover is opened.

- The pre-connected electrodes are stored in the defibrillator cover and can be accessed when the cover is opened.
- A spare set of adult or child electrodes can be found in the compartment at the bottom of the **FRED PA-1**.




#### Adult electrodes 80 cm<sup>2</sup>

The adult electrodes (surface area 80 cm<sup>2</sup>) with the blue connector are used for adult patients (older than 8 years or weighing more than 25 kg).



#### Adult electrodes 80 cm<sup>2</sup> with child adapter

The adult electrodes (surface area 80 cm<sup>2</sup>) with the blue connector and child adapter are used for child patients younger than 8 years old or weighing less than 25 kg and older than 1 year old. The energy setting is automatically reduced when the child adapter is used.



#### Child electrodes 42 cm<sup>2</sup>

The child electrodes with the yellow connector are used for child or infant patients younger than 8 years old or weighing less than 25 kg. The **FRED PA-1** automatically distinguishes between adult electrodes and child electrodes. The energy setting is automatically reduced when child electrodes are connected.

### 4.2.2 Unpacking the electrodes



- ▲ **Risks for the user and the patient.** The packaging of pre-connected electrodes is welded to the electrode cable. Do not remove the packaging from the electrode cable (risk of damaging the cable).
- ▲ Check the expiration date of the electrodes.

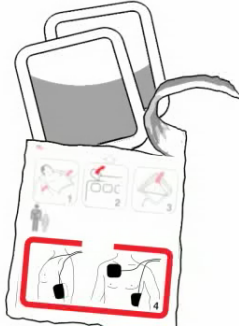


Fig. 4.4 Opening the electrode packaging

During a cardiac arrest, use the **FRED PA-1** on the patient as follows:

- If no emergency services have been alerted, call the local emergency number.
- Switch On the **FRED PA-1** by opening the cover.
- Remove the clothes from the patient's upper body.
- Shave the patient's upper body if necessary.
- Open the electrode packaging carefully.
- If not pre-connected, insert directly the electrode connector into the electrode port of the **FRED PA-1** or in the case of using adult electrodes with the child adapter, firstly insert the electrode connector into the child adapter port and then insert the child adapter connector into the electrode port of the **FRED PA-1**.
- Apply the electrodes to the patient's chest. Refer to section 4.2.3 [Applying the electrodes](#) for the proper placement.




Fig. 4.5 Green indicator

**Notes:**

- The green indicator will blink, and the **FRED PA-1** repeats the instructions until the electrodes are applied or until the electrode connector is connected or until the electrode connector and child adaptor connector is connected, respectively, and the electrode-skin resistance (impedance) has reached an acceptable level.
- If the **FRED PA-1** does not register pad connectivity to the patient, the **FRED PA-1** recommends performing a CPR cycle. The **FRED PA-1** then switches off if it has not detected an acceptable impedance between the two electrodes after 5 minutes.

4.2.3 Applying the electrodes



- ▲ Skin covered in sea water, sand, sunscreen, or skin or body care products may impair electrode contact or cause the electrodes to become disconnected.
- ▲ The skin must be intact.

General indications

Adult electrodes 80 cm<sup>2</sup>



Before applying the adhesive electrodes, check that the application sites on the patient's chest is clean and dry.

1. Carefully shave the application area if the patient's chest is hairy.
2. Apply the electrodes as described below. Do not apply the electrode on top of the clavicle (uneven surface).

The electrodes must have good contact with the patient's skin. Air bubbles under the electrodes must be avoided. To avoid air bubbles, place one edge of the adhesive electrode on the patient's chest, then gradually smooth it out toward the other edge to remove any air.

Place the electrodes on the patient's chest so that the connections point to either side of the patient does not hinder CPR.

**Shown left is the placement of adult electrodes (80 cm<sup>2</sup>) on adult patients (older than 8 years or weighing more than 25 kg).**

The adult electrodes (surface area 80 cm<sup>2</sup>) with the blue connector are used for adult patients (older than 8 years or weighing more than 25 kg).

The electrodes should be in an antero-lateral position.




1. Apply the first electrode, as shown at the right sternal edge at the level of the 2<sup>nd</sup> intercostal space. Do not apply the electrode on top of the clavicle (uneven surface).
2. Apply the second electrode, as shown in the picture, on the left axillary line at the level of the 5<sup>th</sup> intercostal space.

Refer to the picture on the left or to the pictures on the electrode packaging for the correct positioning.


**Placement of adult electrodes (80 cm<sup>2</sup>) on children (1 to 8 years old) weighing less than 25 kg.**

When defibrillating children with adult electrodes (surface area 80 cm<sup>2</sup>) connected or not to the child adapter, it is recommended to choose the antero-posterior position.

The **FRED PA-1** automatically distinguishes between adult electrodes and child electrodes or child adapter. The energy setting is automatically reduced when child pads or child adapter are connected.



Child electrodes 42 cm<sup>2</sup>



**Placement of child electrodes (surface area 42 cm<sup>2</sup>) on child patients weighing less than 25 kg or younger than 8 years old and older than 1 year old.**


The child electrodes (surface area 42 cm<sup>2</sup>) with the yellow connector (see left) are used for child patients weighing less than 25 kg or younger than 8 years old and older than 1 year old.

The **FRED PA-1** automatically distinguishes between adult electrodes and child electrodes. The energy setting is automatically reduced when child pads are connected. The electrodes should be in an antero-lateral position.

1. Apply the first electrode as shown at the right sternal edge at the level of the 2<sup>nd</sup> intercostal space. Do not apply the electrode on top of the clavicle (uneven surface).
2. Apply the second electrode, as shown in the picture on the left axillary line at the level of the 5<sup>th</sup> intercostal space.


Refer to the picture on the left or to the pictures on the electrodes for the correct positioning.

**4.2.4 Connect the adult electrodes with the child adapter**

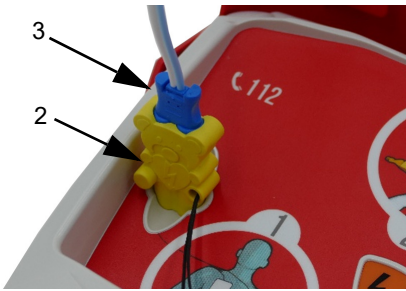

1. Unplug the pre-connected adult electrode.
2. Plug in the child adapter into the **FRED PA-1**.
3. Plug the adult electrode connector into the child adapter.

**4.2.5 Checking the electrodes**



If the resistance (impedance) between the pads and the patient reaches an unacceptable value, the **FRED PA-1** interrupts and prompts the user to check the electrode application; in addition, the green indicator is blinking.

This can occur if:

- The cable is disconnected from the **FRED PA-1**
- The electrodes are not correctly applied to the patient's chest.



In this case, the **FRED PA-1**:

- Prompts to check that the electrodes are connected and applied to the patient's chest and then recommends performing a CPR cycle if no corrective action has been taken.
- Resumes the intervention where it has been interrupted when it detects that the resistance between both electrodes is acceptable again.
- Switches off if it still does not detect acceptable impedance between both electrodes after 5 minutes.

Follow these steps to check the electrodes:

1. Insert the connector as specified in section [3.7.2 Connect the electrodes](#).
2. Press the defibrillation pads onto the patient's chest one after the other to find out which one makes the green indicator switch Off
3. Carefully press this electrode onto the patient's skin
4. If the above steps do not solve the problem, apply new electrodes
  - If you have connected adult electrodes via the child adapter into the **FRED PA-1**, remove and reconnect directly the adult electrodes to the **FRED PA-1**
  - Replace the adult electrodes by child electrodes
  - Change the child adapter
5. If the electrode error remains, perform CPR even if the **FRED PA-1** switches off.



To remove the electrodes from the patient's chest refer to section [4.6 Finishing the Therapy](#).

### 4.2.6 Checking the child adapter



If the resistance (impedance) reaches an unacceptable value, the **FRED PA-1** interrupts and prompts the user to check the electrode application; in addition, the green indicator is blinking.

Refer to section [4.2.5 Checking the electrodes](#)

This can occur:

- When the cable is disconnected from the Child adapter
- If the electrodes are not correctly applied to the patient's chest.
- When the Child adapter is disconnected from the **FRED PA-1**

In this case, the **FRED PA-1**:

- Prompts to check that the electrodes are connected and applied to the patient's chest and then recommends performing a CPR cycle if no corrective action has been taken.
- Resumes the intervention where it has been interrupted when it detects that the resistance between both electrodes is acceptable again.
- Switches off if it still does not detect acceptable impedance between both electrodes after 5 minutes.

Follow these steps to check the electrodes:

1. Insert the connector as specified in section [3.7.2 Connect the electrodes](#) with the child adapter
  - Connect the electrodes.
2. Press the defibrillation pads onto the patient's chest one after the other to find out which one makes the green indicator switch Off
3. Carefully press this electrode onto the patient's skin
4. If the above steps do not solve the problem, apply new electrodes or/and use a new adapter or remove the adapter
5. If the electrode error remains, perform CPR even if the **FRED PA-1** switches off.

To remove the electrodes from the patient's chest (refer to section [4.6 Finishing the Therapy](#)).

## 4.3 Semi-automatic Defibrillation



**Patient hazard**


- ▲ The guidelines given in section [4.1 Instructions and Safety Notes](#) must be observed.



Depending on the configuration, the instructions provided by the **FRED PA-1** may be shortened.

### Step 1

#### Switching on and preparing the FRED PA-1

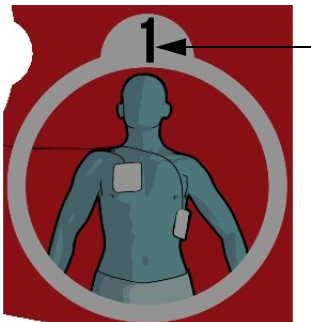

1. Open the cover to switch the **FRED PA-1** On.
  - If the cover is missing, remove the battery and reinsert it to switch the **FRED PA-1** On.
2. Assess the patient's condition: not responsive, no respiration, no pulse.
3. Apply the defibrillation electrodes to the patient's chest (refer to section [4.2 Application of the Adhesive Electrodes](#)).
4. Insert the electrode connector into the electrode port if necessary.
  - Or insert the adult electrode via the child adapter to the **FRED PA-1** if all conditions are met. Refer to section [4.2.1 General information](#)

Fig. 4.6 Apply the electrodes




The **Apply the electrodes** LED blinks for as long as the electrodes are not correctly applied to the patient's chest or the electrode connector is not correctly connected to the **FRED PA-1**.

- Or the electrode connector is not correctly connected to the child adapter port
- Or the child adapter connector is not correctly connected to the **FRED PA-1** port.

### Step 2

#### Analysing the ECG signal

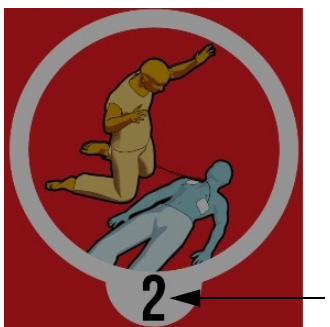

5. The analysis is automatically triggered without user intervention. A message prompts the user not to touch the patient, and the green LED below the pictogram is blinking.

Fig. 4.7 Analysing, do not touch the patient



If the **FRED PA-1** detects VF or VT with a Heart Rate (HR) exceeding 150 bpm, [Step 3 Shock delivery](#) follows; otherwise, continue with [Step 4, Performing CPR](#).

## Step 3

## Shock delivery


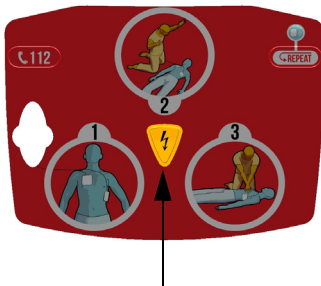



Fig. 4.8 Button to deliver the shock

### Shock hazard

- ▲ Do not, under any circumstances, touch the patient during shock delivery.
- ▲ Check that the patient cannot touch any conducting objects.

Once the analysis has been performed, the **FRED PA-1** charges automatically if a shock is recommended. When the energy is charged, the **Shock** button blinks, and the user is prompted to trigger the shock by pressing the **Shock** button. After the shock, the **FRED PA-1** prompts the user to perform CPR immediately.

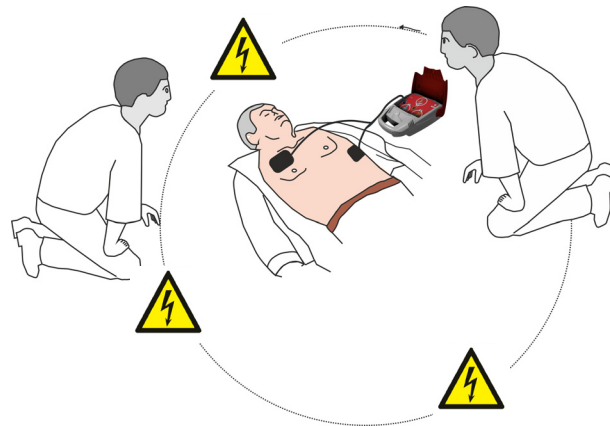

6. Deliver the shock by pressing the **Shock** button   
After the shock delivery, proceed with [Step 4 Performing CPR](#).

## Step 4




## Performing CPR

- ▲ Performing chest compressions can lead to thorax injuries.
- ▲ If the victim is lying on a mattress, chest compressions may be cushioned, leading to a loss in CPR quality. Consider moving the victim on a hard surface for optimal CPR quality.



- In case of difficulty delivering chest compressions at the recommended rate, follow the pace provided by the metronome.
- If the **FreeCPR** option is activated, the **FRED PA-1** instructs the rescuer to adjust the chest compression frequency.
- **FreeCPR** measures the compression rate based on the impedance measurement by the defibrillation electrodes.



7. Perform a CPR cycle. According to the configuration of the **FRED PA-1**, a CPR cycle consists of:
  - Performing chest compressions for the set period of time
  - Alternately performing 30 chest compressions and 2 breaths for the set period of time for adult patients.
  - Alternately performing 15 chest compressions and 2 breaths for the set period of time for child and infant patients.

After the CPR cycle, the **FRED PA-1** continues automatically with [Step 2 Analysing the ECG signal](#).

## Finishing the therapy

Refer to section [4.6 Finishing the Therapy](#)

## 4.4 Automatic Defibrillation



The laws and regulations for the use of automatic defibrillators vary from country to country. While some countries allow laypersons to use automatic defibrillators without any special training, other countries restrict the use of AEDs to EMTs or First Responders who have undergone special training.

### 4.4.1 Functional description of automatic AEDs



Depending on the configuration, the instructions provided by the **FRED PA-1** may be shortened.



Fig. 4.9 FRED PA-1 Automatic

The **FRED PA-1** delivers defibrillation shocks automatically; that is, there is no need to trigger the shock.

Voice prompts and LEDs next to the pictogram keep the user informed regarding the therapy steps.

If a shock is advised, the energy is automatically charged. A countdown accompanies the last 3 seconds before the shock is delivered.

### 4.4.2 Safety notes for automatic defibrillation



#### Risks for patients, users and assistants

- ▲ Once the **FRED PA-1** has been switched on by opening the cover and the electrodes have been applied, the ECG analysis is started automatically, and a shock is delivered automatically if a shockable rhythm is present. The user is informed of an ongoing analysis or shock release via acoustic messages.
- ▲ Touching or transporting the patient during analysis may lead to an incorrect analysis. Analysis results are only valid if the patient remained unconscious during the entire analysis and was not touched.
- ▲ For this reason, chest compressions and artificial respiration must be suspended during the analysis.
- ▲ The patient must not be touched or transported (for example, on a stretcher) during analysis and shock delivery.
- ▲ The notes in section [4.1 Instructions and Safety Notes page 36](#), must be observed.

4.4.3 Automatic defibrillation procedure

Depending on the configuration, the instructions provided by the **FRED PA-1** may be shortened.

Step 1

Switching on and preparing the FRED PA-1

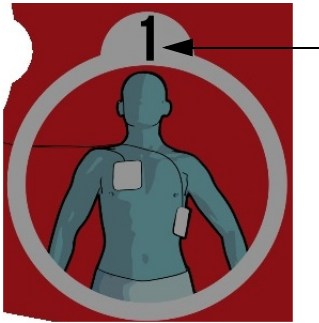


Fig. 4.10 Apply the electrodes

1. Open the cover to switch the **FRED PA-1** On.
  - If the cover is missing, remove the battery and reinsert it to switch the **FRED PA-1** On.
2. Assess the patient's condition: not responsive, no respiration, no pulse.
3. Apply the defibrillation electrodes to the patient's chest (refer to section [4.2 Application of the Adhesive Electrodes](#)).
4. Insert the electrode connector into the electrode port if necessary.
  - Or insert the adult electrode via the child adapter to the **FRED PA-1** if all conditions are met. Refer to section [4.2.1 General information](#)



The **Apply the electrodes** LED blinks for as long as the electrodes are not correctly applied to the patient's chest or the electrodes connector is not correctly connected to the **FRED PA-1**.

- Or the electrode connector is not correctly connected to the child adapter port
- Or the child adapter connector is not correctly connected to the **FRED PA-1** port.

Step 2

Analysing the ECG signal

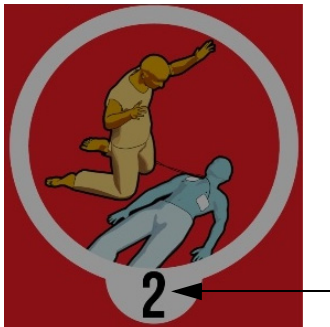


Fig. 4.11 Analysing, do not touch the patient

5. The analysis is automatically triggered without user intervention. A message prompts the user not to touch the patient, and the LED below the pictogram is blinking.



If the **FRED PA-1** detects VF or VT with a HR exceeding 150 bpm, [Step 3 Automatic shock delivery](#) follows; otherwise, continue with [Step 4 Performing CPR](#).

## Step 3


### Automatic shock delivery

**⚠ DANGER**

#### Shock hazard

- ▲ Do not, under any circumstances, touch the patient during shock delivery.
- ▲ Check that the patient does not or cannot touch any conducting objects.

Once the analysis has been performed, the **FRED PA-1** charges automatically if a shock is recommended. As soon as the energy charge is completed, the **FRED PA-1** automatically delivers the shock without user intervention. A verbal countdown starts, and the orange LED blinks until the shock is delivered. After the shock, the **FRED PA-1** prompts the user to perform CPR immediately.

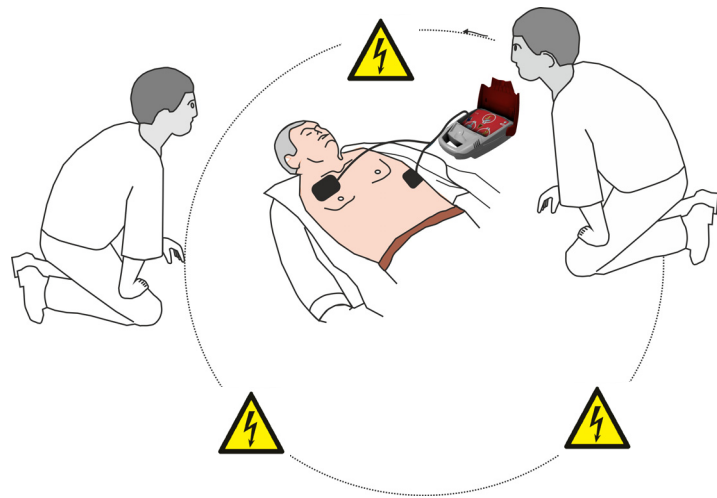

After the shock delivery, proceed with [Step 4 Performing CPR](#).

## Step 4



## Performing CPR

- ▲ Performing chest compressions can lead to thorax injuries.
- ▲ If the victim is lying on a mattress, chest compressions may be cushioned, leading to a loss in CPR quality. Consider moving the victim on a hard surface for optimal CPR quality.



- In case of difficulty delivering chest compressions at the recommended rate, follow the pace provided by the metronome.
- If the **FreeCPR** option is activated, the **FRED PA-1** instructs the rescuer to adjust the chest compression frequency.
- **FreeCPR** measures the compression rate based on the impedance measurement by the defibrillation electrodes.



6. Perform a CPR cycle. According to the configuration of the **FRED PA-1**, a CPR cycle consists of:
  - Performing chest compressions for the set period of time
  - Alternately performing 30 chest compressions and 2 breathes for the set period of time for adult patients.
  - Alternately performing 15 chest compressions and 2 breathes for the set period of time for child and infant patients.

After the CPR cycle, the **FRED PA-1** continues automatically with [Step 2 Analysing the ECG signal](#).

## Finishing the therapy

Refer to section [4.6 Finishing the Therapy](#).

## 4.5 Internal Safety Discharge



- ▲ If the **FRED PA-1** behaviour differs from the description given in this user guide, the **FRED PA-1** is defective and must be repaired.

An internal safety discharge ensures that the stored energy is discharged within the **FRED PA-1** every time a defibrillation shock is not delivered correctly. An internal discharge is performed if:

- The shock has not been delivered within the 20 seconds following the end of defibrillation energy charging
- An electrode error is detected
- The battery voltage is insufficient
- The **FRED PA-1** is defective
- The **FRED PA-1** is switched off before the shock is delivered.

## 4.6 Finishing the Therapy

1. Disconnect the electrode cable.
  - Disconnect the electrode cable from the child adapter and disconnect the child adapter from the **FRED PA-1**.
2. Switch off the **FRED PA-1** once the therapy has been completed (close the cover).
  - If applicable place the child adapter inside the **FRED PA-1** and close the cover.
3. Carefully remove the pads from the patient's skin (refer to [Fig. 4.12 Removing the adhesive pads](#))
4. Discard the disposable pads immediately after use to prevent their reuse (hospital waste).
  - Do not discard nor remove (nor detach) the child adapter: store it back inside the defibrillator cover.
5. Clean the **FRED PA-1**, cables, sensors, and child adapter as described in section [6.2 Cleaning and Disinfecting](#).
6. Connect new electrodes (refer to section [3.7.2 Connect the electrodes](#))
7. Retrieve the intervention data (refer to section [5.1 Retrieving Intervention Data](#))
8. Patients with implanted pacemakers must check the functioning of the pacemaker immediately.

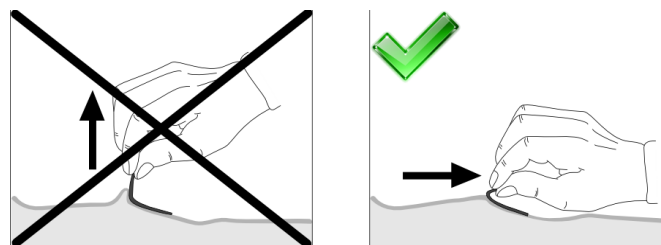


Fig. 4.12 Removing the adhesive pads



If the **FRED PA-1** is turned off for less than 5 minutes, all data is stored (even if the battery is removed). The **FRED PA-1** continues to count the number of shocks delivered, to measure the time elapsed since the **FRED PA-1** was turned on, and to store intervention events from the point at which the **FRED PA-1** was turned off.

## 4.7 Replacing the Battery



1. Close the cover of the **FRED PA-1**.
2. Press the two ends of the battery lock down (1) as indicated to remove the battery.
3. Insert a new battery (refer to section [3.2 Inserting the Battery](#))

# 5 Communication



- ▲ Always follow the Cybersecurity rules in section [1.10 Cybersecurity](#)
- ▲ In case of a bad connection, improve transmission by moving closer to an efficient communication point.

## 5.1 Retrieving Intervention Data


### 5.1.1 For standard FRED PA-1 with an SD card




- Only use standard SD cards (do not use mini or micro SD cards).
- To read the intervention data, use the appropriate SCHILLER software. Contact your SCHILLER representative.

An SD card is required to retrieve the intervention data. The SD card must be configured according to the following instructions.

1. With a computer, create a directory called, *from\_device* on the SD card.
2. Remove the battery from the **FRED PA-1**.
3. Insert the SD card (1).
4. Insert the battery; the **FRED PA-1** is switched on automatically.
5. The modem LED (2) is on, and the service LED (3) is blinking throughout the data transfer process, which can last more than 5 minutes.
6. The data transfer is finalised when the modem LED (1) and the service LED (2) are off.
7. Remove the battery and then remove the SD card from the **FRED PA-1**.
8. Insert the battery.

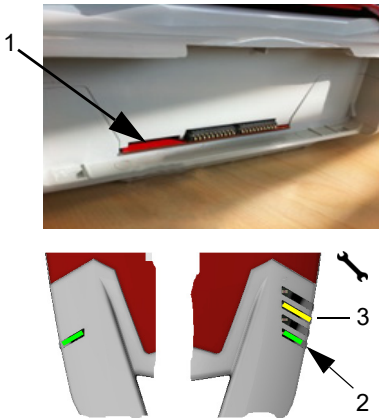

5.1.2 For FRED PA-1 equipped with a cellular network

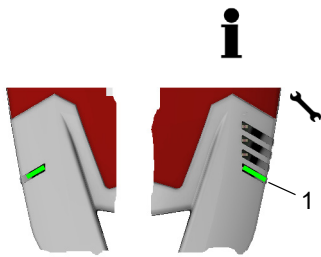

- **FRED PA-1** with the cellular network option is delivered with an embedded SIM card that must not be removed.
- After use on a patient, intervention data is automatically sent to the SCHILLER Server after the next self-test (10 minutes after shutdown).
- Network communication is active while the LifeDataNet G2 service is running, as indicated by the Modem LED (1) blinking shown in the left image.

**FRED PA-1 Management**

**FRED PA-1** is equipped with a cellular network module managed by the SCHILLER Server LifeDataNet G2.

**FRED PA-1** sends information automatically to the server to check, if required that it is operational.



- ▲ The expiration date information stored in the RFID chip of the Adult electrode can not be read by the **FRED PA-1**.
  - Expired adult electrodes might be used.

After each self-test, **FRED PA-1** sends:

- Self-test results
- Battery status
- Pads expiry date. BE CAREFULL, this is not true if you use a child adapter. Indeed, we can use expired adult electrodes with the child adapter, as the RFID chip containing the expiration date is not read by the **FRED PA-1**.
- Alive status

Authorised users can also schedule remote software and configuration updates as well as download log files through the LifeDataNet G2 server. Log files are only used by SCHILLER personnel for investigation.

# 6 Maintenance

## 6.1 Maintenance Intervals



- Because **FRED PA-1** is an emergency device, some verifications are recommended as written in the following table in order to maintain the **FRED PA-1** operational, including the accessories. The test results must be recorded and compared to the values accompanying the documents (refer to section 7.10 [Inspection Report](#))
- Local regulations in your country may stipulate additional or different inspection intervals and tests.
- The following table indicates the intervals and competence of the maintenance work required.
- The user/responsible organisation is responsible for maintaining the device (that is, updating the software/hardware) according to the maintenance interval described below.
- In addition, the user/responsible organisation must update the device according to all manufacturer Field Safety Notices.



- ▲ **Patient hazard.** If the **FRED PA-1** behaviour differs from the description given in this user guide or the RTU LED is not blinking, the **FRED PA-1** is defective and must be repaired.



- ▲ When the **FRED PA-1** is used intensively, SCHILLER recommends shorter intervals between inspections.
- ▲ The regulations in force in each country regarding inspection frequency must be observed (if shorter intervals than those recommended by SCHILLER are imposed).

Interval	Maintenance replacement	Responsible
After each use	<ul style="list-style-type: none"> <li>• Replace the electrodes.</li> <li>• After battery insertion, check that the RTU LED is blinking and that the other LEDs are off (refer to section 6.1.4 <a href="#">RTU LED</a>)</li> <li>• Visual inspection of the <b>FRED PA-1</b> and the child adapter if applicable (refer to section 6.1.3 <a href="#">Visual inspection of the FRED PA-1 and accessories</a>)</li> <li>• Retrieve the intervention data and clear the intervention memory (refer to section 5.1 <a href="#">Retrieving Intervention Data</a>)</li> <li>• Clean and disinfect the <b>FRED PA-1</b> and the child adapter if applicable (refer to section 6.2 <a href="#">Cleaning and Disinfecting</a>)</li> </ul>	→ User
Once a Week	<ul style="list-style-type: none"> <li>• Check that the RTU LED is blinking, and all other LEDs are off (refer to section 6.1.4 <a href="#">RTU LED</a>)</li> <li>• Visual inspection of the <b>FRED PA-1</b>, accessories, and the child adapter if applicable.               <ul style="list-style-type: none"> <li>– If the <b>FRED PA-1</b> has not been used for several weeks, clean and disinfect the <b>FRED PA-1</b> and the child adapter if applicable (refer to section 6.1.3 <a href="#">Visual inspection of the FRED PA-1 and accessories</a>)</li> </ul> </li> </ul>	→ User



**FRED PA-1** equipped with a cellular network module can be exempt from this maintenance interval as long as the **FRED PA-1** is remotely under supervision through the LifeDataNet G2 server.

Interval	Maintenance replacement	Responsible
Every 3 years	<ul style="list-style-type: none"> <li>Perform a software update (if a new version is available).</li> <li>Visual inspection of the <b>FRED PA-1</b>, accessories, and the child adapter if applicable (refer to section <a href="#">6.1.3 Visual inspection of the FRED PA-1 and accessories</a>)</li> <li>Check for correct functioning.</li> <li>Measure the energy delivered at 50 Ohms with the appropriate material.</li> </ul>	→ Service staff authorised by SCHILLER

- Points to inspect**
- Visually inspect the **FRED PA-1**, accessories, and the child adapter if applicable (refer to section [6.1.3 Visual inspection of the FRED PA-1 and accessories](#)).
  - Check for correct functioning.
  - Measure the energy delivered at 50 Ohms.

### 6.1.1 Device status file

**FRED PA-1** can create a file about its current status automatically to help with the maintenance.

The device status file is created every time the **FRED PA-1** is switched on and during each self-test if an SD card is inserted.

The name of the file is written to help identify which **FRED PA-1** it comes from and when it was created. For example:

*SerialNumber\_CurrentDate\_CurrentTime\_device\_status.txt*

The device status file contains several pieces of information, including:

- The current date, that is, when the device status file was created.
- FRED PA-1** serial number
- Next maintenance date
- Package version (of the installed software)
- Status of the electrodes
- Regular battery level as a percentage
- Current alarm list

### 6.1.2 Service and shelf life

**FRED PA-1** The **FRED PA-1** has a defined service life of 10 years if maintenance intervals have been observed according to section [6.1 Maintenance Intervals and the directive IEC/EN 62353](#).

**Battery** Main battery (approximately 6 years); see the expiry date on the battery.

**Electrodes** Electrode packaging (approximately 2 years); see the expiry date on the electrodes pouch.

### 6.1.3 Visual inspection of the FRED PA-1 and accessories

Regularly and after each use, visually inspect the **FRED PA-1**, cables, and the child adapter to detect possible mechanical damages.

If there are any damages or dysfunctions which could endanger the safety of the patient or user, only use the **FRED PA-1** once it has been serviced.

#### Points to inspect

- Check that the RTU LED is blinking and all the other LEDs are off (refer to section [6.5.1 Error messages](#))
  - **FRED PA-1** casing is undamaged
  - No excessive soiling or damages
  - A legible nameplate at the rear of the **FRED PA-1**
  - Legible inscriptions on the front face of the **FRED PA-1**
  - Check the availability of the child adapter (if applicable)
  - Legible inscriptions on the back face of the child adapter if present
  - Child adapter (if applicable) is undamaged
  - The expiration date of the electrodes has not elapsed (refer to section [3.7.2 Connect the electrodes](#))
  - The expiration date of the battery has not elapsed
  - Clean and disinfect the **FRED PA-1** and the child adapter (if applicable) if it has not been used for several weeks (refer to section [6.2 Cleaning and Disinfecting](#)).
- 
- ▲ Electrodes past their expiration date must be replaced immediately (RTU LED is off and the electrodes LED is blinking, only by using the electrodes reference 0-21-0040. This is not true when used with a child adapter as the RFID chip containing the expiration date is not read by the **FRED PA-1**).
  - ▲ Batteries past their expiration date must be replaced immediately (refer to section expiry date on the batteries)
  - ▲ A defective **FRED PA-1** or damaged cables or child adapter must be replaced immediately.
  - ▲ Replace or repair immediately the **FRED PA-1**, if the RTU LED is not blinking (refer to section [6.5.1 Error messages](#))


**6.1.4 RTU LED**

If the **FRED PA-1** is defective or if the **FRED PA-1** has detected problems during the self-test, the **FRED PA-1** must be repaired before use.

If a problem is detected during this self-test:

- An acoustic alarm is issued
- The RTU LED is blinking if a non-critical error is detected as:
  - Battery almost empty
  - Electrode nearly expired (only with electrodes reference 0-21-0040 and not use with the child adapter as the RFID chip containing the expiration date is not read by the **FRED PA-1**).
- The RTU LED is no longer blinking if the **FRED PA-1** is no longer operational
- The corresponding service LED is blinking.

For more details; refer to section [6.5.1 Error messages](#).

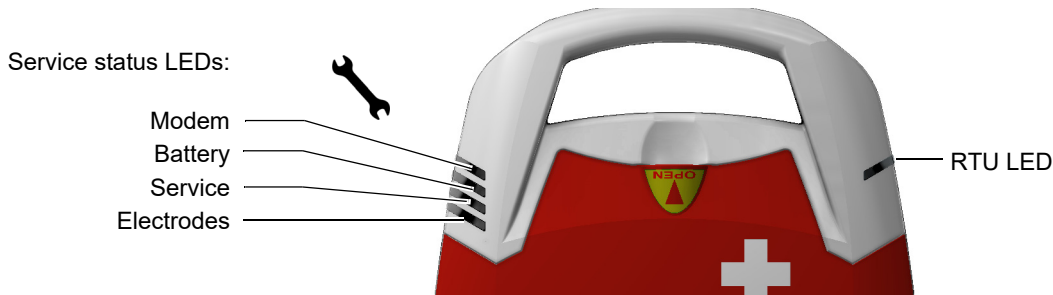

**6.1.5 Maintenance of the non-rechargeable Li/MnO<sub>2</sub> battery**

**Important**

- The battery's performance and life depend on how and under what ambient conditions the battery is used.
- The non-rechargeable battery is maintenance-free during its life.
- The self-discharge of the battery is approximately 1% per year at 25°C. Storage at higher temperatures increases the self-discharge (for example, by approximately 16% per year at 60°C).

**Replacing Li-MnO<sub>2</sub> battery**

- The battery must be replaced when the battery depletion is displayed.
- The battery must be replaced after 6 years from the manufacturing date on the battery.

**Recommendations**

- Store unused batteries at an ambient condition of 20°C ± 5°C.
- Check the battery contacts for corrosion.

## 6.2 Cleaning and Disinfecting



Cleaning removes dust, dirt, and stains; however, this does not constitute a disinfection. Use commercially available detergents intended for clinics, hospitals, and practices.

### 6.2.1 Cleaning detergents

Refer to the manufacturer's information regarding the detergents.

#### Admissible detergents

- Isopropyl alcohol (50%)
- Neutral detergents
- Soap water
- All products that are suitable for ABS0 plastic (housing device), Polycarbonate PC (LCD window) and Polyester PES (keyboard)

#### Non-admissible detergents

Never use products containing the following:

- Ethyl alcohol
- Acetone
- Hexane
- Abrasive cleaning powder
- Plastic dissolving products

### 6.2.2 Disinfection

Use commercially available disinfectants intended for clinics, hospitals, and practices to disinfect the **FRED PA-1** and the child adapter if available. Wipe disinfection removes certain bacteria and viruses. Refer to the manufacturer's information.

#### Admissible disinfectants

- Isopropyl alcohol (50%)
- Propanol (50%)
- Ethyl hexanal
- Aldehyde (2 to 4%)
- Ethanol (50%)
- All products that are suitable for ABS plastics

#### Non-admissible disinfectants

Never use products containing the following:

- Organic solvents
- Ammonia-based detergent
- Abrasive cleaning agents
- 100% alcohol, Virex, Sani-Master
- Sani-Cloth, Ascepti or Clorox wipes
- HB Quat
- Conventional cleaner (for example, Fantastic, Tilex)
- Conductive solution
- Solutions or products containing the following ingredients:
  - Ketone (Acetone)
  - Ammonium chloride
  - Betadine
  - Chlorine, wax, or wax compound
  - Sodium salt

**6.2.3 Cleaning and disinfecting the FRED PA-1, cable, adapter and sensor**



- ▲ **Shock hazard.** Remove the battery before cleaning the **FRED PA-1**. This ensures that the **FRED PA-1** is not turned on inadvertently while you are cleaning it.
- ▲ **Risk of death.** Disconnect the defibrillation pads and adapters before cleaning the **FRED PA-1**.

**Risk of shock and equipment damage.** Liquids must not enter the **FRED PA-1** and the child adapter. If a liquid has penetrated the **FRED PA-1**, it must not be used until a service technician has checked it.



- ▲ Do not immerse the **FRED PA-1**, the cable, the child adapter, or the sensor in liquid and do not sterilise them.
- ▲ Do not apply tension to the sensor cable.
- ▲ Do not use aggressive cleaners.
- ▲ Do not use any phenol-based agents or peroxide compounds for cleaning.
- ▲ Reusable sensors and child adapters must be treated as biologically dangerous material after usage and disinfected according to the manufacturer's instructions.
- ▲ Observe the manufacturer's notes when cleaning the sensors, child adapter and cables.

**Protocols**

1. Remove the battery.
2. Wipe the equipment housing, child adapter, and sensor with a dampened cloth and a mild cleaning solution. The manufacturer recommends using 50% alcohol.
3. Dispose of single-use applied parts and protective coverings according to the relevant regulations.



**Equipment damage**

Do not clean the surface of the **FRED PA-1** or the child adapter with phenol-based disinfectants or peroxide compounds.

**FRED PA-1 casing and child adapter**

Wipe the **FRED PA-1** and the child adapter with a dampened cloth; check that no liquid enters the **FRED PA-1** or the child adapter, especially not into the electrode's pads connector. All cleaning or disinfection products commonly used in hospitals and containing alcohol (maximum 50%) are appropriate.

- If liquids enter the **FRED PA-1**, it can only be operated again after the technical support department has checked it.

**Electrodes**

→ Discard the disposable electrodes immediately after use to prevent their reuse (hospital waste). But do not discard nor detach the child adapter, it is reusable.

## 6.3 Order Information



- ▲ **Risk to persons and equipment damage.** Always use SCHILLER replacement parts and disposables, or products approved by SCHILLER. Failure to do so may endanger life and invalidate the warranty.
- ▲ Using accessories, transducers, adapters and cables other than those specified or provided by the equipment manufacturer could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment, resulting in incorrect operation.

Your local representative stocks all the consumables and accessories for the **FRED PA-1**. A full list of all SCHILLER representatives can be found on the SCHILLER website ([www.schiller.ch](http://www.schiller.ch)). In case of difficulty, contact SCHILLER to process your order or to receive details for all SCHILLER products.

### 6.3.1 Order information

#### Accessories

Part No.	Description
0-21-0040	1 pair of disposable adhesive defibrillation pads for adults, 80 cm <sup>2</sup> ; pre-connected with RFID
2.155067	1 pair of disposable adhesive defibrillation pads for children, 42 cm <sup>2</sup>

### 6.3.2 Consumables and other parts order information

#### Consumables

Part No.	Description
4-07-0025	Battery pack <b>FRED PA-1</b>
5-35-0043	SD Card
0-05-0109	Child adapter

#### Other parts

Part No.	Description
1-127-5180	Wall bracket
6-39-0172	Set of emergency number and flag stickers for <b>FRED PA-1</b>
6-39-0148	Set of emergency number stickers for wall bracket
0-48-0240	User Guide, English

### 6.3.3 Basic package content

- **FRED PA-1**
- User guide
- Sticker sheets
- Pair of adhesive pads
- Li/MnO<sub>2</sub> non-rechargeable battery

## 6.4 Disposal Information

### 6.4.1 Battery disposal



- ▲ Danger of explosion. The battery must not be incinerated, exposed to high-temperatures, or disposed of with household waste.
- ▲ Do not expose the battery to chemicals that could dissolve ABS, polypropylene, polyvinyl chloride, nickel, mylar or steel.
- ▲ Do not cut, destroy, or incinerate the battery.
- ▲ Danger of acid burns. Do not open or heat the battery.
- ▲ Danger of electrolyte leakage. Risk of corrosion.




The battery must be disposed of in municipally approved areas or returned to SCHILLER.

### 6.4.2 Disposal of patient-related accessories



Disposable articles (for example, pads and razors) must be disposed of as hospital waste.

### 6.4.3 Disposal at the end of its useful life



At the end of their service life, the **FRED PA-1** and its accessories must be recycled in compliance with local regulations. Apart from the internal and plug-in batteries, the **FRED PA-1** does not contain hazardous material and can be recycled like any other piece of electronic equipment. In accordance with national law, the battery must be disposed of at an appropriate waste disposal station or returned to SCHILLER.

European legislation has defined that the **FRED PA-1** is considered electronic waste equipment. It can be returned to the distributor or manufacturer, where the **FRED PA-1** is disposed of in compliance with legal requirements. The customer must bear the shipping costs. The **FRED PA-1** must be disposed of in a municipally approved collection point or recycling centre when no longer used.

If no such collection point or recycling centre is available, you can return the **FRED PA-1** to your distributor or the manufacturer for proper disposal. In this way, you contribute to the recycling and other forms of utilisation of old electrical and electronic equipment. Improper disposal harms the environment and human health due to the presence of dangerous substances in electrical and electronic equipment.

## 6.5 Errors and Troubleshooting



- If it is not possible to get the **FRED PA-1** back into operating condition within a reasonable time, continue CPR until the rescue service arrives.

### Forced shutdown procedure


- If the **FRED PA-1** cannot be switched off normally (closing the cover), remove the battery and reinsert it after 10 seconds..

### 6.5.1 Error messages

If a problem is detected during the self-test:

→ Refer to the table below to identify the source of error with the different LEDs.

Service status LEDs:

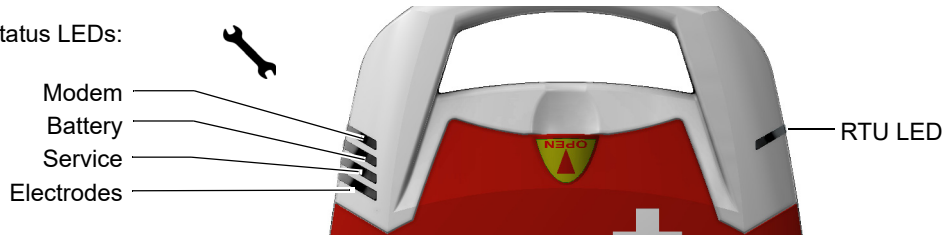

Description	FRED PA-1 state	RTU LED	Alarm sound	Battery LED	Electrode LED	Service LED	Remedy
Power supply problem or corrupted firmware	⊘	○	ON	○	○	○	→ Contact your sales representative.
Battery pack defect	⚠	○	ON	●	○	○	→ Replace the battery
The main battery is almost empty (lower than 10%), or the battery's shelf life has expired.	✓	●	OFF	●	○	○	→ Replace the battery
First case: the electrodes expire within 2 months. Second case: no RFID defibrillation pads are detected (configuration).	✓	●	OFF	○	●	○ or ●	→ First case: Replace the electrodes → Second case: During the last test, no electrodes were detected. Check the connection of the pre-connected electrodes and the child adapter if present. Start a new test or wait for the next periodic test.
Electrodes expiration date exceeded	✓	○	OFF	○	●	○	→ Replace the electrodes, remove the battery and reinsert it.
<b>FRED PA-1</b> needs a service	✓	●	OFF	○	○	●	→ Contact your sales representative.
Service delay expired	✓	○	OFF	○	○	●	→ Contact your sales representative.
<b>FRED PA-1</b> is out of order	⚠	○	ON	○	○	●	→ Replace the <b>FRED PA-1</b>



Normal **FRED PA-1** state. The **FRED PA-1** is fully operational. A defibrillation shock can be given.

Restricted **FRED PA-1** state. The **FRED PA-1** is not able to charge the HV capacitor and deliver a defibrillation shock. It only indicates that CPR should be performed.



Critical **FRED PA-1** state. The **FRED PA-1** is out of order.

### 6.5.2 General errors and troubleshooting



#### Forced shutdown procedure

If the **FRED PA-1** cannot be switched off normally (closing the cover), remove the battery and reinsert it after 10 seconds.

Problem	Possible causes	Remedy
The status indicator is not blinking and the <b>FRED PA-1</b> cannot be turned on.	<ul style="list-style-type: none"> <li>Battery defect.</li> <li>No battery inserted, or battery not correctly inserted.</li> <li><b>FRED PA-1</b> is defective.</li> </ul>	<ul style="list-style-type: none"> <li>→ Replace the battery.</li> <li>→ Insert the battery correctly.</li> <li>→ Have the <b>FRED PA-1</b> repaired.</li> </ul>
The status indicator is blinking, and the <b>FRED PA-1</b> cannot be turned on.	<ul style="list-style-type: none"> <li><b>FRED PA-1</b> cover is missing</li> </ul>	<ul style="list-style-type: none"> <li>→ Remove the battery and reinsert it to start the <b>FRED PA-1</b> into the resuscitation process.</li> </ul>
The <b>FRED PA-1</b> prompts the user to check that the electrodes are properly applied and connected.	<ul style="list-style-type: none"> <li>Short-circuit between the pads.</li> <li>Poor pad contact.</li> <li>Electrodes connector, not connected to the <b>FRED PA-1</b></li> <li>Dry contact agent.</li> <li><b>FRED PA-1</b> is defective.</li> </ul>	<ul style="list-style-type: none"> <li>→ Apply the pads exactly as described.</li> <li>→ Firmly press down on the pads.</li> <li>→ Connect the electrodes to the <b>FRED PA-1</b></li> <li>→ Connect the electrodes via the child adapter to the <b>FRED PA-1</b></li> <li>→ Use new electrodes.</li> <li>→ Have the <b>FRED PA-1</b> repaired.</li> </ul>
The <b>FRED PA-1</b> cannot be turned off.	<ul style="list-style-type: none"> <li>Close the cover</li> <li>Software hangs</li> <li><b>FRED PA-1</b> is defective.</li> </ul>	<ul style="list-style-type: none"> <li>→ Hold down the cover so that the magnetic sensor is activated</li> <li>→ Remove the battery and reinsert it.</li> <li>→ Have the <b>FRED PA-1</b> repaired.</li> </ul>
Incorrect analysis result (for example, the <b>FRED PA-1</b> does not detect a shockable rhythm, even though the patient exhibits VF).	<ul style="list-style-type: none"> <li>Insufficient ECG signal quality.</li> <li>Electromagnetic waves disturb the ECG signal.</li> <li>Patient moved during analysis.</li> <li><b>FRED PA-1</b> is defective.</li> </ul>	<ul style="list-style-type: none"> <li>→ Repeat chest compressions.</li> <li>→ Turn Off the source of interference (for example, radio transmitter or cellular telephone). Position the patient outside the range of interference.</li> <li>→ Do not move the patient during the analysis.</li> <li>→ Have the <b>FRED PA-1</b> repaired.</li> </ul>
Defibrillation shock cannot be delivered.	<ul style="list-style-type: none"> <li>Insufficient battery charge level.</li> <li>CPR caused pads error.</li> <li><b>FRED PA-1</b> is defective.</li> </ul>	<ul style="list-style-type: none"> <li>→ Replace the battery.</li> <li>→ Re-apply the pads.</li> <li>→ Check that the pads are properly connected via the child adapter to <b>FRED PA-1</b></li> <li>→ Have the <b>FRED PA-1</b> repaired.</li> </ul>
The alarm tone does not stop.	<ul style="list-style-type: none"> <li>Battery defect.</li> <li><b>FRED PA-1</b> is defective.</li> </ul>	<ul style="list-style-type: none"> <li>→ Replace the battery.</li> <li>→ Have the <b>FRED PA-1</b> repaired.</li> </ul>
Battery LED is On.	<ul style="list-style-type: none"> <li>Battery almost depleted.</li> </ul>	<ul style="list-style-type: none"> <li>→ Replace the battery.</li> </ul>

Problem	Possible causes	Remedy
No data was recorded on the SD card.	<ul style="list-style-type: none"><li>• Card defect.</li><li>• <b>FRED PA-1</b> is defective.</li></ul>	<ul style="list-style-type: none"><li>→ Replace the card.</li><li>→ Have the <b>FRED PA-1</b> repaired.</li></ul>
The electrodes LED continue to blink even after replacing the electrodes	<ul style="list-style-type: none"><li>• Alarms are not reset</li></ul>	<ul style="list-style-type: none"><li>→ Remove the battery and reinsert it to force a test</li></ul>
Difficulty to insert the battery	<ul style="list-style-type: none"><li>• Protective cap not removed</li></ul>	<ul style="list-style-type: none"><li>→ Remove the contacts protective cap</li></ul>
The <b>FRED PA-1</b> does not start the automatic test by inserting a battery	<ul style="list-style-type: none"><li>• The battery contacts are dirty</li><li>• The battery is empty</li></ul>	<ul style="list-style-type: none"><li>→ Clean the battery contacts with an alcohol-dampened cloth</li><li>→ Use a new battery</li></ul>

## 6.6 Electromagnetic Interference

### 6.6.1 Measures to prevent electromagnetic interferences



Non-ionising electromagnetic radiation

Precautions must be taken to prevent adverse events to the Patient and the Operator due to electromagnetic disturbance.

The user can help avoid electromagnetic disturbances by keeping the minimum distance between portable and mobile HF telecommunication devices (transmitters) and the **FRED PA-1**. The minimum distance of 0.3 meter has been tested according to IEC 60601-1-2 for a wide range of telecommunication equipment, as shown in the following table:

HF Source	Transmitter frequency [MHz]	Power P [W]	Distance d [m]
Radiotelephone (microcellular) CT1+, CT2, CT3	885-887	0.010	0.23
Cordless DECT telephone, WLAN, UMTS phone	1880-2500	0.25	1.17
Mobile phone USA	850/1900	0.6	1.8
Mobile phone - GSM900, - GSM850, NMT900, DCS 1800	900 850,900,1800	2 1	3.3 2.3
Walkie-talkie (rescue service, police, fire brigade, service)	81-470	5	2.6
Mobile telephone system (rescue service, police, fire brigade service)	81-470	100	11.7
RFID (active and passive transponders and reading devices)	433 865-868	0.5	0.85 1.62



- ▲ Portable HF telecommunication devices must not be used within a radius of 0,3 meter from the **FRED PA-1**, its cables and child adapters.
- ▲ Do not place the **FRED PA-1** on top of other electric/electronic devices; that is, maintain a sufficient distance from other devices (this includes the patient cables).
- ▲ Avoid using AED nearby power lines and generators for the railway networks countries with frequency of 16 2/3 Hz, like Switzerland, Germany, Austria, Sweden, Norway

For permanent HF telecommunication devices (for example, radio and TV), the recommended distance can be calculated using the following formula:

$$d = 1.2 \times \sqrt{P} \text{ for } 150 \text{ kHz to } 800 \text{ MHz and } d = 2.3 \times \sqrt{P} \text{ for } 800 \text{ MHz to } 2.7 \text{ GHz,}$$

with:

d = Recommended minimum distance in Meters

P = Transmitting power in Watts



For more information on operation in an electromagnetic environment according to IEC/EN 60601-1-2; refer to the Service manual.

### 6.6.2 Additional measures

The user can take the following measures to prevent electromagnetic interferences:

- Increase distance to the source of interference.
- Turn the device **FRED PA-1** to change the angle of radiation.
- Only use original accessories and consumables (especially defibrillation electrodes)
- The device **FRED PA-1** should not be used adjacent to or stacked with other equipment.
- Observe the maintenance intervals as stated in [6.1 Maintenance Intervals](#).



- ▲ Use of the **FRED PA-1** adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, the **FRED PA-1** and the other equipment should be observed to verify that they are operating normally.
- ▲ Using accessories, transducers, consumables, and cables other than those specified or provided by the equipment manufacturer could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in incorrect operation.
- ▲ However, there is no guarantee that no interference can occur in certain installations. If the **FRED PA-1** causes interferences, these can be prevented by switching off the **FRED PA-1**.



For more detailed information; refer to section [7.6 Telecommunication \(options\)](#)

# 7 Technical Data



Unless otherwise stated, all specifications are valid at a temperature of 25°C.

## 7.1 System Specifications

<b>Manufactured by</b>	SCHILLER MEDICAL
<b>Device name</b>	<b>FRED PA-1</b>
<b>Dimensions</b>	310 x 255 x 100 mm (h x l x w)
<b>Weight</b>	Approximately 2.5 kg with battery and standard accessories
<b>Protection class of the device housing</b>	IP55 (protection against dust and water jets)
<b>Recorded data</b>	ECG signal recording (2 hours) Technical events (500 events)
<b>Power supply</b>	
<b>Battery type</b>	Lithium/MnO <sub>2</sub> 15V, 2.8 Ah
Battery life	The power supply is suitable for continuous operation for 4 hours and 30 minutes with intermittent loading or more than 140 shocks at maximum energy if the <b>FRED PA-1</b> is stored/used in optimal temperature conditions between 15 to 25°C.
Standby duration	For a standard <b>FRED PA-1</b> with an SD card <ul style="list-style-type: none"> <li>• Several years in standby: Standby duration corresponding to laboratory tests at 25°C: 6 years with weekly self-tests.</li> </ul> For the <b>FRED PA-1</b> with cellular network <ul style="list-style-type: none"> <li>• Several years in standby: Standby duration corresponding to laboratory tests at 25°C, with a constant, good cellular network connection and without antenna roaming: 3 years with weekly self-tests.</li> </ul>
<b>Environmental conditions</b>	
<b>Device</b>	
Operation	<ul style="list-style-type: none"> <li>• 0 to 40°C at a relative humidity of 30 to 95% (non-condensing)</li> <li>• Atmospheric pressure 700 to 1060 hPa (approximately 3000 to -400 meters).</li> </ul>
Storage before use	<ul style="list-style-type: none"> <li>• 0 to 40°C with the battery inserted and including electrodes at a relative humidity of 30 to 95% (non-condensing); however, this may result in a reduced battery life. Optimal conditions are 15 to 25°C to ensure maximum battery life.</li> <li>• Atmospheric pressure 700 to 1060 hPa</li> </ul>
Storage and transport	<ul style="list-style-type: none"> <li>• -20 to 50°C at a relative humidity of 30 to 95% (non-condensing)</li> <li>• Atmospheric pressure 700 to 1060 hPa</li> </ul>
<b>Battery, child adapter, and electrodes</b>	

- |   |  |
|---|--|
| Operating temperature battery<br>LiMnO <sub>2</sub>   | • 0 to 60°C  |
| Storage and operating temper-<br>ature electrode pads | • 0 to 50°C  |
| Storage and operating temper-<br>ature child adapter  | • 0 to 50°C  |
| Transport temperature elec-<br>trodes pads            | • Maximum of 10 days between -40 to 0°C and 50 to 75°C |
-

## 7.2 Classification and Safety Standards

### Standards

**FRED PA-1** complies with IEC standard 60601-2-4. In compliance with the requirements of IEC standard 60601-2-4, the **FRED PA-1** is a device for infrequent use.

### EMC

Refer to Chapter 7 [Technical Data](#)

### Compliance

- The **FRED PA-1** bears the CE-0459 mark (Notified Body GMED), indicating its compliance with the general safety and performance requirements of Annex I of the Medical Device Regulation (EU) 2017/745 regarding safety, functionality, and labelling. The requirements apply to patients, users and third parties who come into contact with this device within the scope of its intended use.
- **FRED PA-1** is a class III device.

### Patient Protection

BF type, resistant to defibrillation shocks.

### Explosions protection

**FRED PA-1** is not designed to be used in the presence of flammable mixtures of anaesthetic agents with air or oxygen.

The SCHILLER quality management system complies in full with the international standard ISO 13485.

## 7.3 Defibrillation Pulse

In the case of prolonged use, particular attention must be paid to the condition of the electrodes. Electrodes must be changed if they become detached or if you receive a message about an electrode defect during the procedure.

In the case of frequent use, particular attention must be paid to the condition of the child adapter. The child adapter must be changed if it deteriorates prematurely deteriorated (trace of cuts, tears) or if the message concerning defective electrodes while using the connector is recurrent/persistent.

### Waveform

Biphasic truncated exponential waveform with variable phase duration for impedance compensation. The impedance range for shock delivery is 25 to 250 Ohms ( $\Omega$ )


### Accuracy of delivered energies

Below is a table showing the accuracy of the measured delivered energy for each couple of most of the rated delivered energies and impedance values of 25 to 175  $\Omega$  is the required range for impedance compensation as required by the IEC 60601-2-4 standard.

Rated delivered energy Joules (J)	25 $\Omega$	50 $\Omega$	75 $\Omega$	100 $\Omega$	125 $\Omega$	150 $\Omega$	175 $\Omega$
10 J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J
15 J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J
20 J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J	$\pm 3$ J
30 J	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$
50 J	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$
100 J	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$
150 J	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$
200 J	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$	$\pm 15\%$


### Graphical plots

The waveform shape is delivered currently in the function of time in milliseconds for different impedances ranging from 25 to 175  $\Omega$  at 200 joules selected energy.

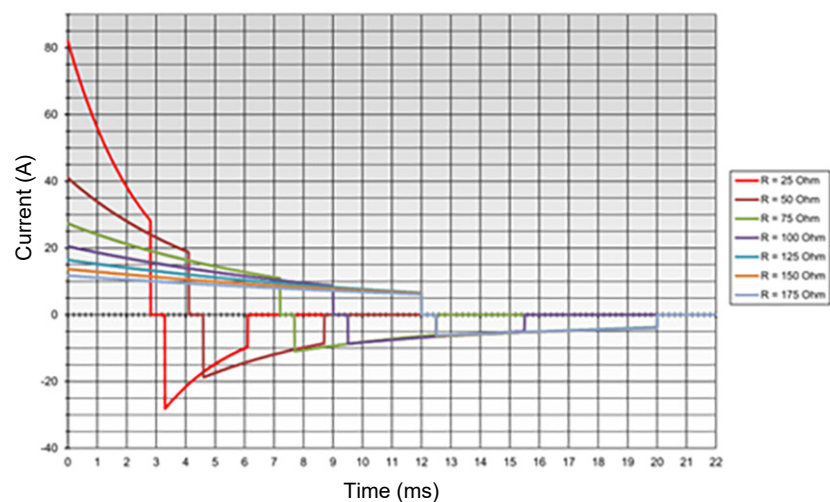


Waveform shape of delivered current in the function of time in milliseconds for

different impedances ranging from **25 to 175 Ω** at **50 joules** selected energy.

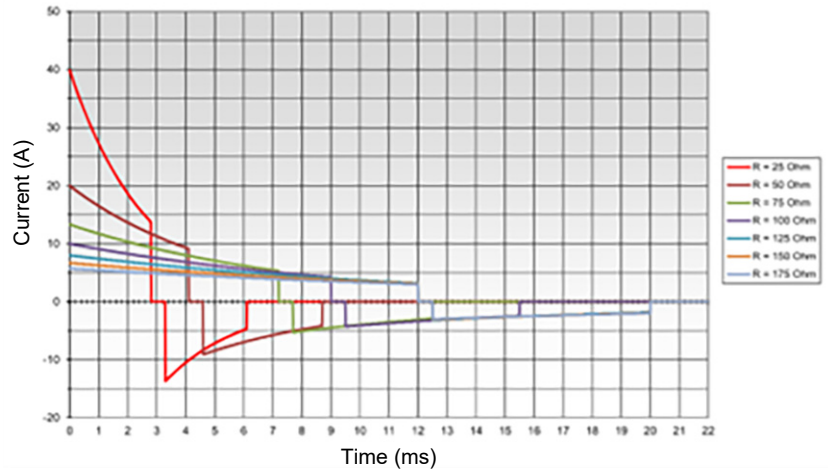

Delivered energy output curves in function of patient impedance. Each curve corresponds to a rated energy selection.

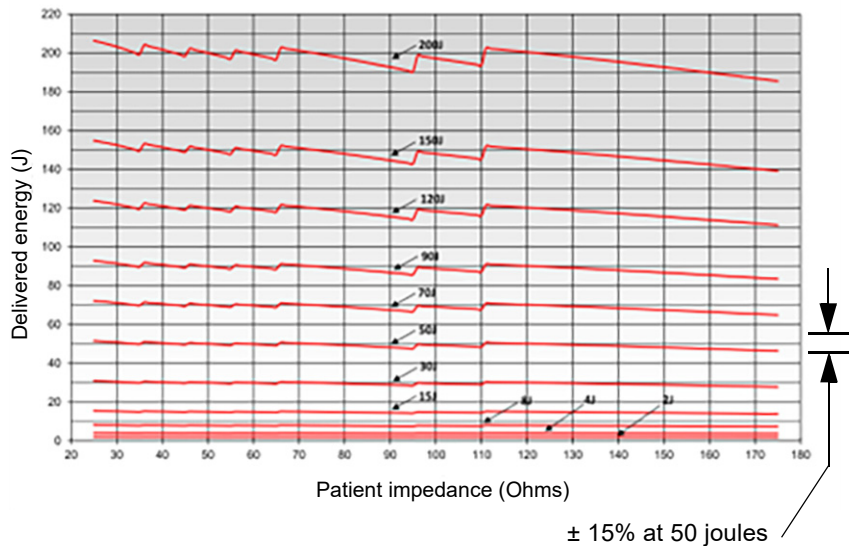

**Default energy settings**

- SCHILLER's customer service department can change the default energy levels to the following values:
  - 90 –120 – 150 – 200 joules (Adults)
  - 30 – 50 – 70 joules (Child)
 (Automatic adaptation when child pads or adult pads via the child adapter are connected)

**Cycle time: from initially switching power on to ready for discharge.**

For AEDs, the maximum time from initially switching power on to ready for discharge, in semi-automatic mode at a maximum energy of 200 joules with a non-rechargeable battery for infrequent use.

After 6 discharges at maximum energy:

- < 29 seconds

---

**Cycle time: rhythm analysis – shock availability (in semi-automatic mode)**

With a new fully charged battery:  
After 6 discharges at maximum energy:

For AEDs, the maximum time the initiation of rhythm analysis with a clear ECG signal to readiness for discharge, in semi-automatic mode at a maximum energy of 200 joules with a non-rechargeable battery for infrequent use.

- < 10 seconds
- < 10 seconds

**Capacitor charging time**

With a new fully charged battery:  
After 6 discharges at maximum energy:  
After 15 discharges at maximum energy:

The maximum charging time of the capacitor, in semi-automatic mode, at a maximum energy of 200 joules with a non-rechargeable battery for infrequent use.


- < 10 seconds
- < 10 seconds
  
- < 10 seconds

Note: the charging of the capacitor is made during the analysis step.


**Patient impedance at which shock delivery is possible**

25 to 250  $\Omega$  (Impedance is compensated up to 200  $\Omega$ )

**Indication when ready to shock**

The orange button  is lit

**Shock delivery**

- With the orange button  (in semi-automatic)
- Using disposable pads applied to the patient in an antero-lateral or antero-posterior position

**Safety discharge when:**

- A non-shockable rhythm has been detected
- The shock is not delivered within 20 seconds after charging
- An electrode problem is detected
- Battery voltage is insufficient
- The **FRED PA-1** is defective
- The **FRED PA-1** is turned off.

**Defibrillation pad connection**

BF type

**Defibrillation electrodes**

Electrode cable, 2 meters in length

Adult pads:

- 80 cm<sup>2</sup> active surface area

Child pads:

- 42 cm<sup>2</sup> active surface area
-

## 7.4 Shock Advisory System (SAS)

### SAS validation process

SCHILLER's AEDs are highly sophisticated, microprocessor-based devices embedding a Shock Advisory System (SAS) that analyse multiple features of the electrical signal (ECG) received from the patient's heart. The ECG signal is acquired via the defibrillation electrode pads, usually in antero-lateral or also called sterno-apical position (equivalent to a lead II ECG). For child or infant patients (under 8 years old), the antero-posterior position of the defibrillation pads is recommended. SCHILLER's AEDs are thought to be operated by rescuers who do not need to recognise or interpret heart rhythms. For this reason, the SAS is an essential component of the AED.

An SAS should recommend:

- A shock if the analysed rhythms is a lethal ventricular arrhythmia, either a VF or a rapid VT hi
- No shock for non-shockable ECG rhythms.

Detailed descriptions of the shockable/non-shockable rhythms categories are given in the following section.

A rhythm analysis by the SAS is requested and is run automatically and periodically after each CPR period. In some AED models, the operator needs to press a button to initiate the rhythm analysis. A rhythm analysis requires from 5 to 10 seconds, depending on the SAS configuration.

The performance of the SAS embedded in SCHILLER's AEDs is evaluated on two criteria: Sensitivity (Se) and Specificity (Sp). Se refers to the AED's ability to detect life-threatening ventricular arrhythmias. Sp refers to the AED's ability to detect normal sinus rhythms or arrhythmias that should not be shocked.

The American Heart Association (AHA) task force published a consensus document [1] reflecting the views of the AHA scientific members on AED's SAS validation. This document is intended to supplement existing AED SAS performance requirements from the IEC standard [2].

Validation database:

The process of validation of SAS uses two independent ECG signal databases, one for learning and one for validation.

Each database is composed of recordings from holter systems and SCHILLER nMedical AEDs. Moreover, each database includes both adult, child and infant recordings.

The diagnostic bandwidth of holter signals (0,05 to 150 Hz) has been limited to (0,5 to 30 Hz) so that the frequency content of the signals is typical of the one found in SCHILLER Medical AED recordings.

Validation Databases (DB)	Recording method	Patient type	Number of patients	Number of 10-second ECG segments
PhysioNet MIT-VFDB [6]	Holter	Adult	21	567
IH DB	Holter	Children 7 years IQR (5 to 8) years	47	69
OHCA DB	SCHILLER's AED FRED EASY	Adult	733	1132
OHCA DB	SCHILLER's AED FRED EASY	Children and infants 8 years IQR (6M to 16) years	188	275
All DBs			989	2043

**Table 1: Summary of ECG databases used for SAS validation**

- **MIT-VFDB:** MIT-BIH Malignant Ventricular Arrhythmia Database, and is a subset of the general PhysioNet database recognised as standard in ECG tests.
- **IH:** Intra-Hospital
- **OHCA:** Out-Of-Hospital Cardiac Arrest

**ECG annotations**

The rhythm annotation is performed by expert observation of 10-second ECG segments/strips (one ECG channel). At least three expert decisions (for example, emergency physicians, experienced cardiologists, electrophysiologists, and biomedical engineers) are combined for a consensus rhythm annotation. The rhythm annotation follows the AHA classification scheme [1], defining the following rhythm types:

Shockable rhythms:

- VF as coarse VT (> 200  $\mu$ V peak-to-peak amplitude)
- VT hi as rapid VT (HR > 150 bpm, rushes that last more than 8 seconds)

Non-shockable rhythms:

- Asystole as asystole (peak-to-peak amplitude  $\leq$  100  $\mu$ V) during more than 4 seconds
- NSR as Normal Sinus Rhythm (P-QRS-T waves visible, HR > 40 bpm and HR < 100 bpm)
- N as other non-shockable rhythm (includes all rhythms except those in other listed categories, for example, Atrial Fibrillation/Flutter (AF), Sinus Bradycardia (SB), Supraventricular Tachycardia (SVT), Premature Ventricular Contractions (PVCs), Heart Blocks (HB), as mentioned in [1].

Intermediate rhythms:

- VT lo as other VT (HR > 40 bpm and < 150 bpm, more than 3 rushes)
- Fine VF as fine VF (peak-to-peak amplitude > 100  $\mu$ V and  $\leq$  200  $\mu$ V) during more than 4 seconds.

**SAS performance**

The performance of SAS shown in the tables below is above expectations according to AHA recommendations [1] and IEC standards [2]. Thereby, SCHILLER AEDs embedded SAS are effective and safe to be used on patients.

The performance of the algorithm is evaluated by comparing the SAS decision with the consensus diagnosis of three expert annotators.

An interpretation table is built and shows:

- The True Positive (TP), that is, a correct classification of a shockable rhythm;
- The True Negative (TN), that is, a correct classification of a non-shockable rhythm (Asystole or N or NSR)
- The False Positive (FP), that is, a non-shockable rhythm (Asystole or N or NSR) that has been incorrectly classified as a shockable rhythm;
- The False Negative (FN), that is, a VF or VT hi that has been incorrectly classified as non-shockable;
- The Sensitivity (Se) of the device for shockable rhythms is:
  - $Se_{VF} = TP/(TP + FN)$ , applied to VF rhythms
  - $Se_{VT\ hi} = TP/(TP + FN)$ , applied to VT hi rhythms
- The True Predictive value (TPv), that is, the probability that a shock is needed when the AED recommends it:
  - $TPv = (TP)/(TP + FP)$  applied to both VF and VT hi results
- The Specificity (Sp) of the device for non-shockable rhythms is:
  - $Sp_{NSh} = TN/(FP + TN)$
- The False Positive rate (FPr) is:
  - $FPr = FP/(FP + TN)$ , applied to non-shockable rhythms

The test sample sizes proposed per category reflect a balance between reasonable confidence in performance and realistic limits on data available to demonstrate it. The minimum sample sizes defined to reach significant results may be exceeded. One parameter to measure this significance is the 90% single-sided lower confidence limit (LCL90%). For each rhythm category, the LCL90% should be calculated based on test results. This process provides a 90% probability that the actual performance is greater than the lower confidence limit calculated. In other words, this value indicates if the computed Se and Sp have a low enough disparity in accordance with the number of analysed segments. For each category, the observed test results, Se, Sp and LCL90%, must equal or exceed the performance goal.

Rhythms	Minimum test sample size	Test sample size	Performance goal		Observed performance	
			Se, Sp (%)	LCL 90%	Se, Sp (%)	LCL 90%
VF	200	571	Se > 90%	> 87%	Met [1]	Met [1]
VT hi	50	213	Se > 75%	> 67%	Met [1]	Met [1]
NSR	100	118	Sp > 99%	> 97%	Met [1]	Met [1]
N	30	452	Sp > 95%	> 88%	Met [1]	Met [1]
Asystole	100	634	Sp > 95%	> 92%	Met [1]	Met [1]
<b>Intermediate rhythms</b>						
VT lo	25	26	Report only	Report only	> 10% shocked	N/A
Fine VF	25	29	Report only	Report only	> 40% shocked	N/A

**Table 2: Performance for SAS (VFDetectClean V2.031) as required by AHA (Artifact Free ECG samples) [1]**

NA: Not Applicable

	VF	VF hi	Non-shockable rhythms (NSR/N/Asystole)
Shock	546	204	9
No shock	25	9	1195
Performance goal	Se > 90%	Se > 75%	Sp > 95%
Observed performance	Met [2]	Met [2]	Met [2]
<b>Additional performance without a goal</b>			
True predictive value	> 90%		N/A
False positive rate	N/A		< 5%

**Table 3: Performance for SAS (VFDetectClean V2.031) as required by IEC standard (Artifact Free ECG samples) [2].**

### **SAS configuration**

The SAS embedded in the device can be configured as Analysis with anteriority. This SAS setting uses a combination of algorithms, which are launched in two stages, (3 - 5) to deliver a shock-advisory decision at minimal delay after the end of chest-compressions. The SAS configured as Analysis without anteriority starts a chest compression-free VF detection at an analysis request without trying to optimise hands-off time. In both configurations, the SAS does not continue analysing after a shock advised decision is reached.

### **References**

- [1]: Kerber, R. E., L. B. Becker, J. D. Bourland, R. O. Cummins, A. P. Hallstrom, M. B. Michos, G. Nichol, et al. 1997. « Automatic external defibrillators for public access defibrillation: recommendations for specifying and reporting arrhythmia analysis algorithm performance, incorporating new waveforms, and enhancing safety. A statement for health professionals from the American Heart Association Task Force on Automatic External Defibrillation, Subcommittee on AED Safety and Efficacy ». *Circulation* 95 (6): 1677-82.
- [2]: Standard IEC 2010 60601-2-4, ed 3.
- [3]: Didon, Jean-Philippe, Vessela Krasteva, Sarah Menetre, Todor Stoyanov, et Irena Jekova. 2011. « Shock Advisory System with Minimal Delay Triggering after End of Chest Compressions: Accuracy and Gained Hands-off Time ». *Resuscitation, Proceedings of the Eleventh Wolf Creek Conference*, 82 (décembre): S8-15. [https://doi.org/10.1016/S0300-9572\(11\)70145-9](https://doi.org/10.1016/S0300-9572(11)70145-9).
- [4]: Didon, Jean-philippe, Irena Jekova, Sarah Ménétré, Todor Stoyanov, et Vessela Krasteva. 2011. « Abstract 219: Combination of Algorithms to Decrease Preshock Pause for Automated External Defibrillators ». *Circulation* 124 (suppl\_21): A219-A219. [https://doi.org/10.1161/circ.124.suppl\\_21.A219](https://doi.org/10.1161/circ.124.suppl_21.A219).
- [5]: Didon, Jean-philippe, Sarah Menetre, Irena Jekova, et Vessela Krasteva. 2010. « Abstract 253: Method for Minimal Delay Triggering of VF Detection During Cardio Pulmonary Resuscitation ». *Circulation* 122 (suppl\_21): A253-A253. [https://doi.org/10.1161/circ.122.suppl\\_21.A253](https://doi.org/10.1161/circ.122.suppl_21.A253).
- [6]: Greenwald, Scott D. 1992. « The MIT-BIH Malignant Ventricular Arrhythmia Database ». [physionet.org. https://doi.org/10.13026/C22P44](https://doi.org/10.13026/C22P44).

## 7.5 Configuration Settings



### Important

- Modifications that can be made via software programs are only performed if requested by the customer or if required by legal requirements.
- These modifications need to be registered in the **FRED PA-1** documentation as well as communicated to all users.

SCHILLER's service centre can configure the following parameters:

- Selection of the default language at **FRED PA-1** start
- The energy level for the 1<sup>st</sup>, 2<sup>nd</sup> and 3<sup>rd</sup> shock (separate settings for adults and children)
- Number of chest compressions for children (15 or 30)
- Self-test frequency (daily or weekly)
- Choose between **continuous chest compressions** or **alternating chest compressions/breaths** during CPR cycles.
- Date and time
- Update of the software
- Change of the **FRED PA-1** language
- Selection of the AED protocol (short or long instructions)
- Activation of notification if no RFID defibrillation pads are detected
- Activation of notch filter (50 to 60 Hz)
- Activation of 16,7 Hz Filter
  - The 16.7 Hz filter must be enabled when the **FRED PA-1** is installed in railway stations.
- Activation of visual notification in case of elapsed maintenance interval (frequency of service can be custom between 1 to 10 years).
- The volume

## 7.6 Telecommunication (options)

<b>Module</b>	LE910C1-WWX
<b>Frequency range</b>	836 MHz (TX) and 882 MHz (RX/IDLE) – 4G Band 5 1950 MHz (TX) and 2140 MHz (RX/IDLE) – 4G Band 1
<b>Supported SIM cards</b>	3 and 1.8V
<b>Data transmission</b>	LTE Cat. 1 <ul style="list-style-type: none"> <li>• Uplink up to 5 Mbps</li> <li>• Downlink up to 10 Mbps</li> </ul>
<b>Maximum transmitting power</b>	<ul style="list-style-type: none"> <li>• 4G LTE – Class 3 (0.2 Watt)</li> </ul>
<b>FCC identification IC ID</b>	<ul style="list-style-type: none"> <li>• R17LE910C1</li> <li>• 5131A-LE910C</li> </ul>
<b>Standards</b>	<ul style="list-style-type: none"> <li>• FCC/IC, PTCRB, ISED</li> <li>• RED/GCF</li> </ul>

## 7.7 Electromagnetic Interferences

The **FRED PA-1** is intended for use in the electromagnetic environment specified below. The customer or the user of the **FRED PA-1** should ensure that it is used in such an environment.

### 7.7.1 Electromagnetic emissions

Emission measurement	Compliance with the regulations	Electromagnetic environment explanations
RF emissions CISPR 11	Group 1	<b>FRED PA-1</b> uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	<b>FRED PA-1</b> is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonics IEC 61000-3-2	Not applicable	
Voltage fluctuations IEC 61000-3-3	Not applicable	

### 7.7.2 Electromagnetic immunity

Interference testing	IEC 60601 test level	Conformity level	Electromagnetic environment explanations
Electrostatic discharge IEC 61000-4-2	± 8 kV contact ± 15 kV air	IEC 60601-1 conformity	Floors should be made of wood, concrete or ceramic tiles. If floors are covered with synthetic material, relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	± 2 kV for power supply lines ± 1 kV for input/output lines	Not applicable	No mains power is used
Surge IEC 61000-4-5	± 1 kV between conductors ± 2 kV conductor-earth	Not applicable	No mains power is used
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	< 5% $U_T$ (> 95% dip in $U_T$ ) for 0.5 cycle 40% $U_T$ (60% dip in $U_T$ ) for 5 cycles 70% $U_T$ (30% dip in $U_T$ ) for 25 cycles < 5% $U_T$ (> 95% dip in $U_T$ ) for 5 seconds	Not applicable	No mains power is used
Power frequency (50 to 60 Hz) magnetic field IEC 61000-4-8	3 A/m	IEC 60601-1 conformity	Power frequency magnetic fields should be that of a typical commercial or hospital environment.

Note:  $U_T$  indicates the AC voltage of the mains before the test level.

Interference testing	IEC 60601 test level	Conformity level	Electromagnetic environment explanations
----------------------	----------------------	------------------	--

Conducted HF IEC 61000-4-6	3 V <sub>eff</sub> between 150 kHz and 80 MHz outside of the ISM frequency bands <sup>a</sup>	Not applicable	No mains power is used
	10 V <sub>eff</sub> between 150 kHz and 80 MHz in ISM frequency bands <sup>a</sup>	Not applicable	

Recommended minimum distances  
Portable and mobile HF telecommunication devices must keep the recommended minimum distance from the **FRED PA-1** and all its components, including cables and child adapters; the recommended minimum distance is calculated based on the transmitter's frequency.

$$d = \frac{12}{10} \times \sqrt{P} \quad \text{Between 80 and 800 MHz}$$

$$d = \frac{23}{10} \times \sqrt{P} \quad \text{Between 800 MHz and 2.5 GHz}$$

Where P is the maximum transmitting power of the transmitter in Watts (W) according to manufacturer data, and d is the recommended minimum distance in metres (M)<sup>b</sup>.

Radiated HF IEC 61000-4-3	10 V/m 80 MHz to 2.5 GHz	10 V/m
------------------------------	--------------------------	--------

The field strength of stationary HF transmitters (according to an on-location measurement<sup>c</sup>) must not exceed the conformity level for each frequency range<sup>d</sup>.

When operating the device near devices bearing the symbol "ionising radiation", interferences can occur.



Non-ionising electromagnetic radiation

Note 1: For 80 to 800 MHz, the higher frequency range applies.

Note 2: These guidelines might not always be applicable. Electromagnetic radiation is influenced by absorption and reflection on structures, objects and people.

- a. The ISM frequency bands (ISM = industrial, scientific, medical) between 150 kHz and 80 MHz are 6.765 to 6.795 MHz, 13.553 to 13.567 MHz, 26.957 to 27.283 MHz, and 40.66 to 40.70 MHz.
- b. The conformity levels within the ISM frequency bands between 150 kHz and 80 MHz and between 80 MHz and 2.5 GHz serve to minimise the probability of interferences caused by mobile/portable communication equipment that accidentally happens to be in the patient's environment. The formula for the calculation of the recommended distance has been adapted by the factor 10/3 for transmitters in this frequency range.
- c. The field strength of stationary transmitters, for example, base stations for radio telephones (mobile or cordless) and portable radio equipment, amateur radios, AM and FM radios and TV signals, cannot be predicted accurately in a theoretical way. In order to analyse electromagnetic environments caused by stationary HF transmitters, an electromagnetic analysis on-site should be considered. If the measured field strength exceeds the HF conformity level, it needs to be checked whether the FRED PA-1 can be used in this environment. If an abnormal behaviour is detected, additional measures need to be taken, for example, reorientation or change of location of the FRED PA-1.
- d. For the frequency range between 150 kHz and 80 MHz, the field strength must be lower than 3 V/m.

### 7.7.3 Recommended minimum distances

The **FRED PA-1** is intended to be used in electromagnetic environments in which it is possible to control radiated HF interferences. The user of the **FRED PA-1** can prevent electromagnetic interferences by always keeping a minimum distance between portable/mobile HF communication devices (transmitters) and the **FRED PA-1**. The recommended minimum distances are listed in the following table according to the transmitters' maximum transmitting power.

Maximum transmitting power of the transmitter (W)	Distances according to the transmitter's frequency (m)			
	$d = \frac{3,5}{3} \times \sqrt{P}$ Between 150 kHz and 80 MHz <b>outside of</b> the ISM frequency band	$d = \frac{12}{10} \times \sqrt{P}$ Between 150 kHz and 80 MHz <b>within</b> the ISM frequency band	$d = \frac{12}{10} \times \sqrt{P}$ Between 80 and 800 MHz	$d = \frac{23}{10} \times \sqrt{P}$ Between 800 MHz and 2.5 GHz
0,01	Not applicable	Not applicable	0,12	0,23
0,1			0,38	0,73
1			1,2	2,3
10			3,79	7,27
100			12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in Metres (M) can be determined using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in Watts (W) according to the transmitter manufacturer.

Note 1: At 80 and 800 MHz, the separation distance for the higher frequency range applies.

Note 2: The ISM (industrial, scientific, and medical) bands between 150 kHz and 80 MHz are 6,765 to 6,795 MHz, 13,553 to 13,567 MHz, 26,957 to 27,283 MHz, and 40,66 to 40,70 MHz.

Note 3: An additional factor of 10/3 has been incorporated into the formula used in calculating the recommended separation distance for transmitters in the ISM frequency bands between 150 kHz and 80 MHz and in the frequency range 80 MHz to 2,5 GHz to decrease the likelihood that mobile/portable communications equipment could cause interference if it is inadvertently brought into patient areas.

Note 4: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

## 7.8 Literature

<b>European Resuscitation Council</b>	Guidelines 2015 for Cardiopulmonary Resuscitation and Emergency Cardiovascular Care
<b>American Heart Association</b>	Guidelines 2015 for Cardiopulmonary Resuscitation and Emergency Cardiovascular Care

## 7.9 Glossary

<b>ABCD</b>	The primary ABCD A = Airways (check if the airways are free) B = Breathing (artificial respiration) C = Circulation (circulatory signs or cardiac massage) D = Defibrillation
<b>AED</b>	Automated External Defibrillator. This term is also used for semi-automatic defibrillators.
<b>BLS</b>	Basic Life Support (artificial respiration and cardiac massage) CPR is frequently used synonymously.
<b>CPR</b>	Cardiopulmonary Resuscitation
<b>VT</b>	Ventricular Tachycardia
<b>VF</b>	Ventricular Fibrillation

## 7.10 Inspection Report



The user guide must be read before the inspection.

Serial number: \_\_\_\_\_

### Checks after each use

→ Check that the green indicator is blinking and all the other LEDs are Off (refer to section 6.1.4 RTU LED)	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
→ Visual inspection of the <b>FRED PA-1</b> , consumables, and accessories					
→ The <b>FRED PA-1</b> casing is undamaged.					
→ The child adapter is available and undamaged	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
→ No excessive soiling or damage	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
→ Legible nameplate at the rear of the <b>FRED PA-1</b>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
→ Legible inscriptions on the front face of the <b>FRED PA-1</b>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
→ Expiration date of the accessories has not elapsed	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<b>Date:</b>					
<b>Performed by:</b>					

### Checks once a Week or Month

<b>Visual inspection of the FRED PA-1, consumables, and accessories</b> (see previous table)	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
The RTU LED (1) is lit green, and no other LEDs are blinking (refer to section 6.1.4 RTU LED)	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<b>Date:</b>					
<b>Performed by:</b>					



### Checks every 3 years

<b>Visual inspection of the FRED PA-1, consumables, and accessories</b> (see previous table)	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<b>Functional test</b>					
→ Check for proper functioning (refer to section 6.1.4 RTU LED)	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
→ Measure the energy delivered at 50 Ohms.	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<b>Date:</b>					
<b>Performed by:</b>					

In case of problems, notify your Biomedical Department  your local SCHILLER distributor  or the authorised Customer Service for your area

Name: .....

Tel: .....



# 8 Index

## A

Accessories .....	64
Appendix	
Glossary .....	85
Inspection Report .....	86
Literature .....	85
Order information .....	84
Required accessories .....	64

## B

Basic package content .....	64
Battery	
Battery Disposal .....	65
Battery is empty .....	33
Inserting the battery .....	28
Low battery .....	32
Sufficient battery capacity .....	32
Biocompatibility .....	21

## C

Cleaning .....	62
Consumables .....	64
Consumables and other parts order information .....	64
Controls and indicators	
Display .....	25

## D

Danger of explosion .....	28
Defibrillation	
Automatic defibrillation .....	50
Defibrillator application guidelines .....	36
Finishing the therapy .....	54
Internal safety discharge .....	54
Semi-automatic Defibrillation .....	47
Design .....	22
Disinfection .....	62
Display Symbols/Indicators	
In this User Guide .....	15
On the display .....	17
On the electrode packaging .....	18
Used on the battery .....	17
Used on the device .....	16
Disposal information	
Accessories into contact with patients ..	65
At the end of useful life .....	65
Battery .....	65

## E

Electrodes	
Adult and child electrodes .....	43
Checking the child adapter .....	46
Checking the electrodes .....	45
Open the electrode packaging .....	42

## F

Function .....	24
----------------	----

## M

Maintenance	
Internal backup battery .....	62
Maintenance Intervals .....	58
Test .....	62
Visual inspection .....	60

## O

Order Information	
Accessories .....	64
Consumables .....	64
Other parts .....	64
Other parts .....	64

## S

Safety Notes .....	7
Symbols and Indicators	
Symbols used in this user guide .....	15
Symbols used on the batteries .....	17
Symbols used on the child adapter packaging .....	20
Symbols used on the electrode packaging .....	18
Symbols used on the FRED PA-1 .....	16


















## T





















Technical Data	
Defibrillation impulse .....	74
Dimensions .....	71
Energy levels .....	75
Environmental conditions .....	71
Patient impedance .....	76
Patient Protection .....	73
Power supply .....	71
Protection class .....	71
Standards .....	73
Weight .....	71
Terms of warranty .....	14
Troubleshooting .....	66

# 13 Appendix - Symbols

This appendix lists all general symbols that may be present on the device, label and accessories. Not all of those symbols are necessarily present on your device.






This appendix has its own article number, which is independent of the user guide's article number.

	Manufacturer information
	Country of manufacturer
	Manufacturing date
	Distributor
	Importer
	Authorised Representative in the Switzerland/United Kindom
	Authorised Representative in the European Community
	CE marking, affirms its conformity with European standards
	Notified body (e.g.  0459 marking notified body GMED)
	UKCA marking (UK Conformity Assessed)
	Regulatory Compliance Mark for the Australian standards
	NRTL symbol (Nationally Recognised Testing Laboratory) TÜV SÜD as accredited NRTL certification provider
	Medical device
	Reference number
	Serial number
	Batch code

	UDI: unique device identification as QR code machine readable and human readable as number (e.g.  (01) 0 761 3365 00210 2 (21)xxxx.xxxxxx )
	Global Trade Item Number
	Quantity
	EIP = electronic information product (does not contain any toxic and hazardous substances or elements above the maximum concentration values (product can be recycled and re-used))
	Electrical and electronic equipment. The device must not be disposed of in the household waste
	Battery. Battery must not be disposed of with domestic refuse
	Direct current
	Alternating current
	Fuse
	Positioning of primary battery
	Rechargeable battery
	Do not dispose in fire
	Do not deform or damage
	Do not open or dismantle
	Do not short circuit
	Do not charge
	Non-ionizing electromagnetic radiation. To indicate that the device contains a Radio Frequency (RF) transmitter to transmit data (e.g. Bluetooth or WiFi)
	Universal Serial Bus (USB) port/plug
	Contains a Bluetooth module

	Read the instruction for use
	Monitor
	Defibrillator
	Humidity limitation for storage and transport, respectively
	Atmospheric pressure limitation for storage and transport, respectively
	Temperature limit for storage and transport, respectively
	Keep dry
	Keep away from sunlight
	Do not re-use
	Do not use if package is damaged
	Fragile, handle with care
	Handle with care
	Transport upwards (This way up)
	Expiry date (for battery, electrodes or other consumables)
	Packaging unit
	Eco packaging
	The unit/component can be recycled
	Recyclable/renewable – Low-density polyethylene
	Warning

13 Appendix – Symbols

	<p>For electrical hazards, warning or precautionary measures when dealing with electricity</p>
	<p>Dangerous voltage. Used for electrical dangers during defibrillation</p>
	<p>Use no hooks</p>
	<p>BF symbol. The device signal input is defibrillation protected</p>
	<p>Signal input type CF. Highly isolated port, defibrillation protected. However, it is only defibrillation protected when used with the original SCHILLER patient cable</p>
<p>IPXX</p>	<p>Ingress Protection Code</p>